

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072115\
 Data File : BE090184.D
 Acq On : 20 Jul 2015 20:41
 Operator : TP/IZ
 Sample : SSTD3.215
 Misc :
 ALS Vial : 7 Sample Multiplier: 1


Quant Time: Jul 21 05:09:20 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE072115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 21 03:09:00 2015
 Response via : Initial Calibration




Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	877	0.40	ng/ul	0.00
2) Naphthalene-d8	10.37	136	4515	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.21	164	2540	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.94	188	6504	0.40	ng/ul	0.00
16) Chrysene-d12	21.11	240	7731	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	6365	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	0.00	152	0d	0.00	ng/ul	
14) Fluoranthene-d10	0.00	212	0d	0.00	ng/ul	
Target Compounds						
11) Pentachlorophenol	16.60	266	2470	3.91	ng/ul	Qvalue 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072115\
Data File : BE090184.D
Acq On : 20 Jul 2015 20:41
Operator : TP/IZ
Sample : SST3.215
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Jul 21 05:09:20 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE072115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 21 03:09:00 2015
Response via : Initial Calibration

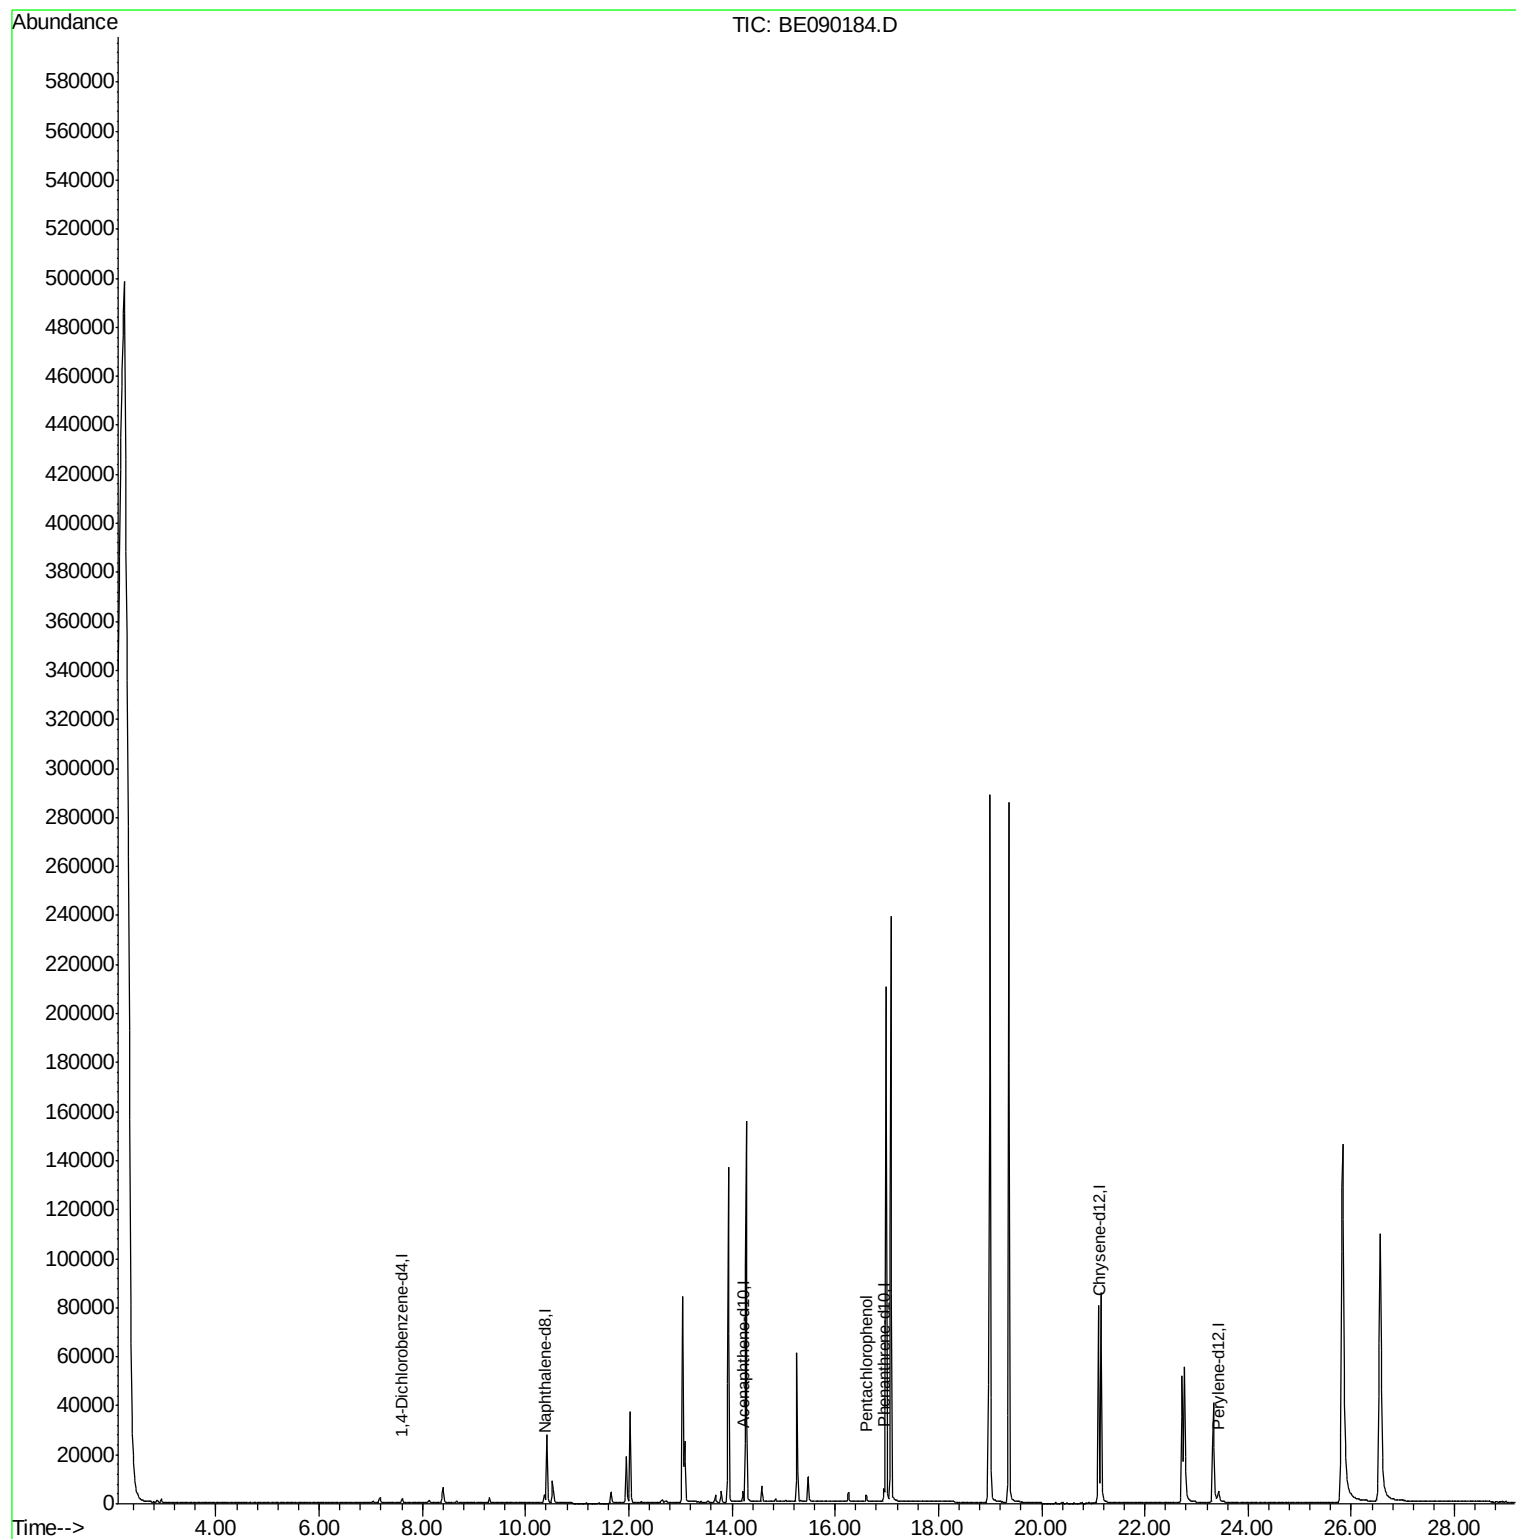

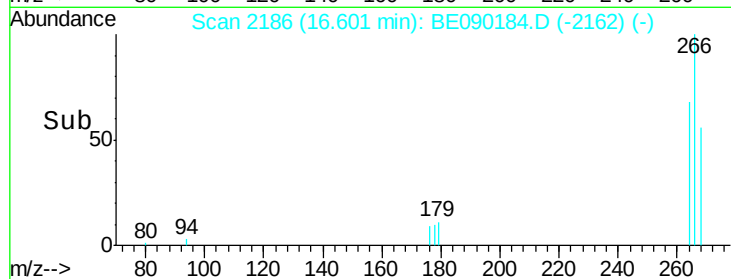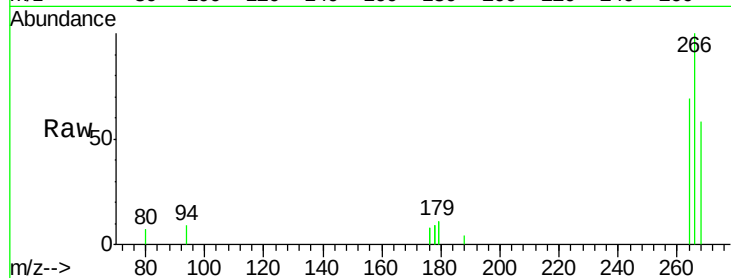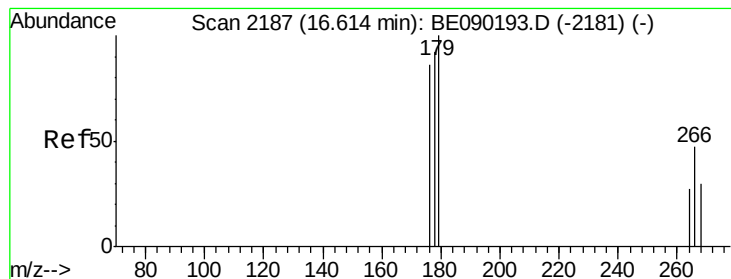

#11
 Pentachlorophenol
 Concen: 3.91 ng/ul
 RT: 16.60 min Scan# 2186
 Delta R.T. -0.01 min
 Lab File: BE090184.D
 Acq: 20 Jul 2015 20:41

Tgt Ion: 266 Resp: 2470
 Ion Ratio Lower Upper
 266 100
 264 64.3 47.7 71.5
 268 65.2 47.0 70.6

