


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072115\
Data File : BE090178.D
Acq On : 20 Jul 2015 16:57
Operator : TP/IZ
Sample : DFTPP03
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE072115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 21 07:09:07 2015

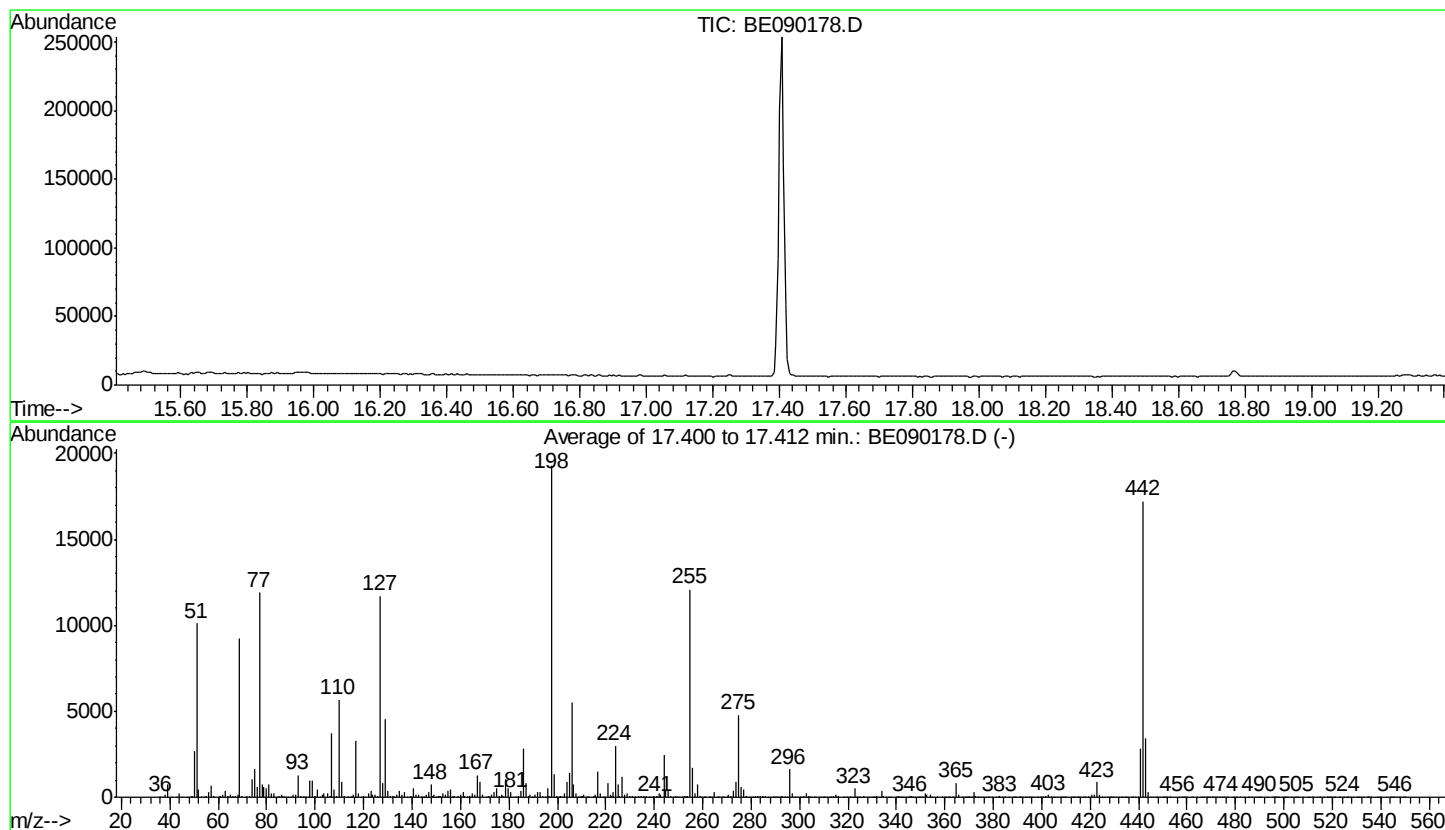

AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.4	10108	PASS
68	69	0.00	2	1.4	125	PASS
69	198	0.00	100	47.8	9225	PASS
70	69	0.00	2	0.8	70	PASS
127	198	10	80	60.6	11700	PASS
197	198	0.00	2	0.2	42	PASS
198	198	100	100	100.0	19293	PASS
199	198	5	9	7.0	1355	PASS
275	198	10	60	24.8	4783	PASS
365	198	1	100	4.3	822	PASS
441	443	0.01	100	82.5	2831	PASS
442	198	50	100	89.2	17217	PASS
443	442	15	24	19.9	3430	PASS