


#1




1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.93 min Scan# 403  
Delta R.T. 0.00 min  
Lab File: BE093505.D  
Acq: 21 Jul 2017 12:31

Instrument :  
BNA\_E  
ClientSampleId :

Tgt Ion: 152 Resp: 2749  
Ion Ratio Lower Upper  
152 100  
150 141.9 125.1 187.7  
115 64.7 55.7 83.5

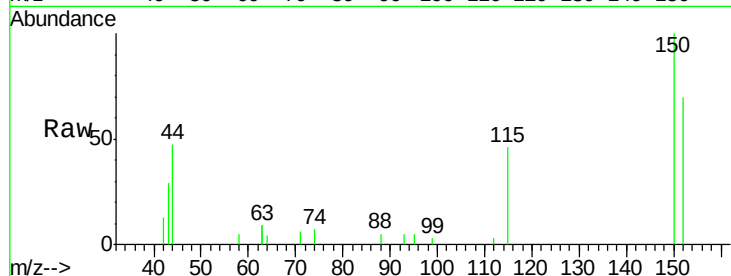


Abundance Ion 152.00 (151.70 to 152.70): E  
Ion 150.00 (149.70 to 150.70): E  
Ion 115.00 (114.70 to 115.70): E

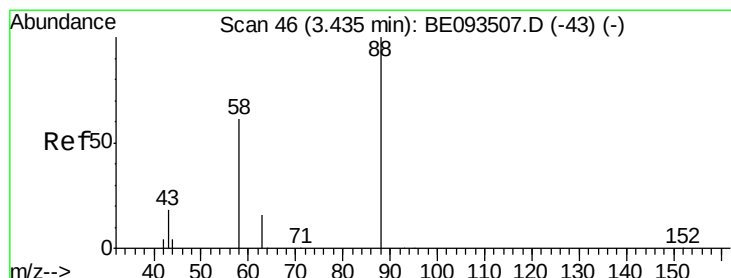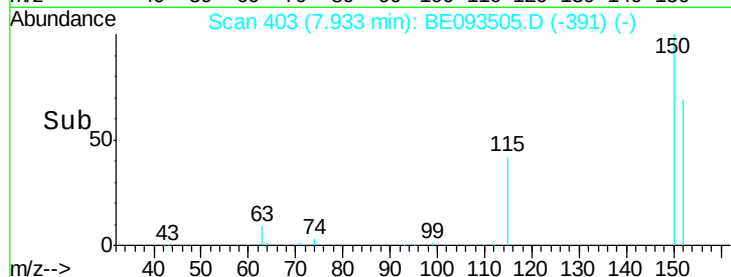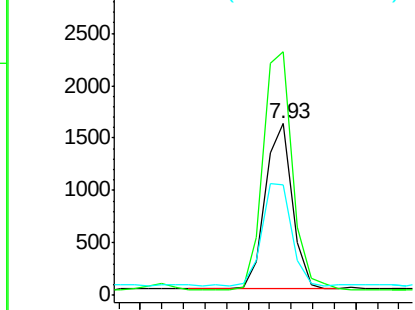

#2

1,4-Dioxane  
Concen: 0.093 ng  
RT: 3.44 min Scan# 46  
Delta R.T. 0.00 min  
Lab File: BE093505.D  
Acq: 21 Jul 2017 12:31

Tgt Ion: 88 Resp: 542  
Ion Ratio Lower Upper  
88 100  
58 71.6 62.2 93.4  
43 64.9 23.2 34.8#

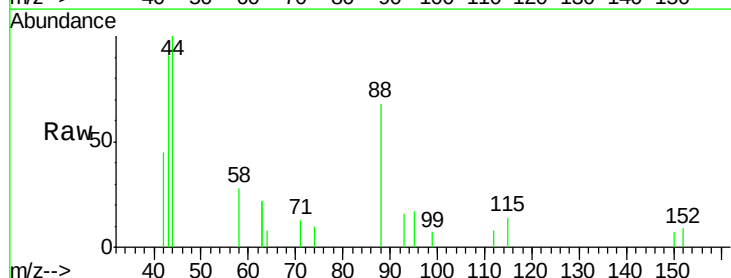

Abundance Ion 88.00 (87.70 to 88.70): BE0  
Ion 58.00 (57.70 to 58.70): BE0  
Ion 43.00 (42.70 to 43.70): BE0

