

#5

Phenol-d6

Concen: 0.115 ng

RT: 7.09 min Scan# 336

Delta R.T. -0.01 min

Lab File: BE093505.D

Acq: 21 Jul 2017 12:31

Instrument :

BNA_E

ClientSampleId :


Tgt Ion: 99 Resp: 1404

Ion Ratio Lower Upper

99 100

42 17.8 0.0 0.0#




71 32.3 0.0 0.0#

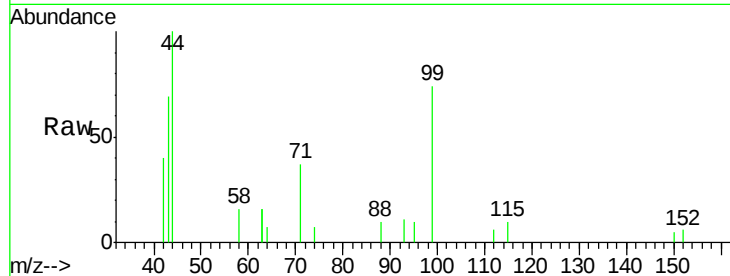

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

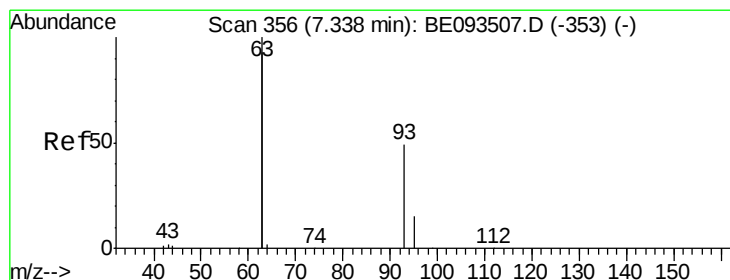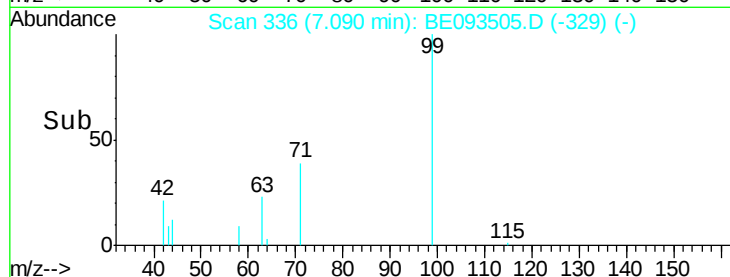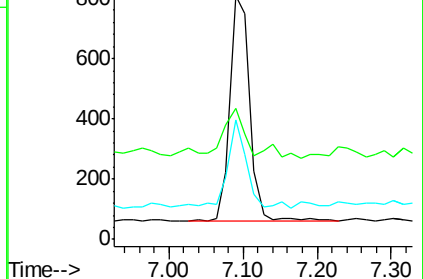

#6

bis(2-Chloroethyl)ether

Concen: 0.115 ng

RT: 7.34 min Scan# 356

Delta R.T. 0.00 min

Lab File: BE093505.D

Acq: 21 Jul 2017 12:31


Tgt Ion: 93 Resp: 1060

Ion Ratio Lower Upper

93 100

63 321.2 0.0 0.0#

95 35.6 25.4 38.0

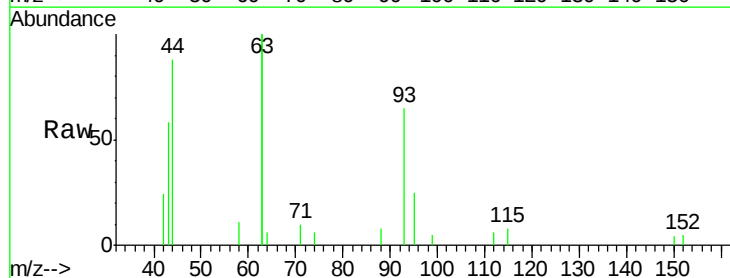

Abundance Ion 93.00 (92.70 to 93.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

Ion 95.00 (94.70 to 95.70): BE0

