





#15
2-Fluorobiphenyl
Concen: 0.108 ng
RT: 13.16 min Scan# 1019
Delta R.T. -0.00 min
Lab File: BE093505.D
Acq: 21 Jul 2017 12:31

Instrument :
BNA_E
ClientSampleId :

Tgt Ion:172 Resp: 3302
Ion Ratio Lower Upper
172 100
171 34.9 29.8 44.6
170 23.6 20.7 31.1

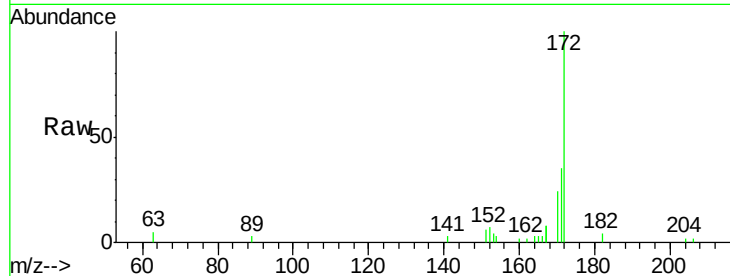


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

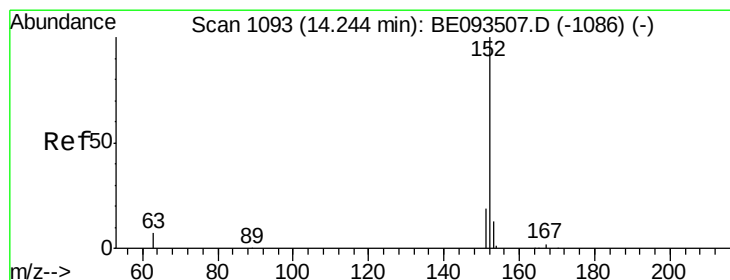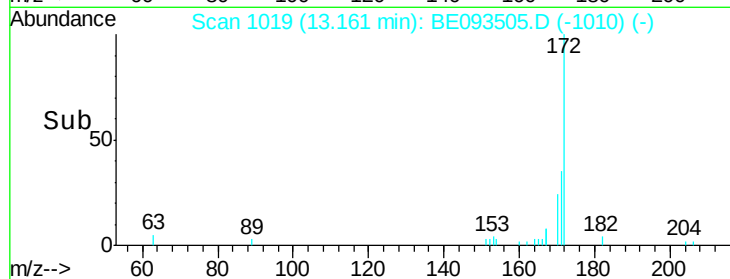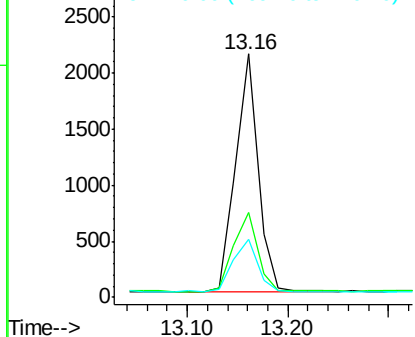

#16
Acenaphthylene
Concen: 0.118 ng
RT: 14.24 min Scan# 1092
Delta R.T. -0.00 min
Lab File: BE093505.D
Acq: 21 Jul 2017 12:31

Tgt Ion:152 Resp: 3879
Ion Ratio Lower Upper
152 100
151 20.6 4.0 6.0#
153 13.1 10.3 15.5

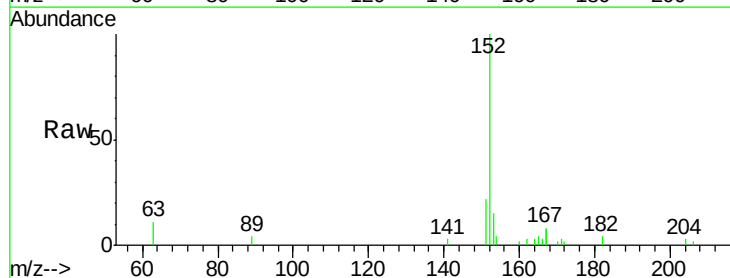

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E
Ion 153.00 (152.70 to 153.70): E

