





#17
Acenaphthene
Concen: 0.110 ng
RT: 14.58 min Scan# 1115
Delta R.T. -0.00 min
Lab File: BE093505.D
Acq: 21 Jul 2017 12:31

Instrument :
BNA_E
ClientSampled :

Tgt Ion:154 Resp: 2653
Ion Ratio Lower Upper
154 100
153 115.8 91.2 136.8
152 53.5 44.8 67.2

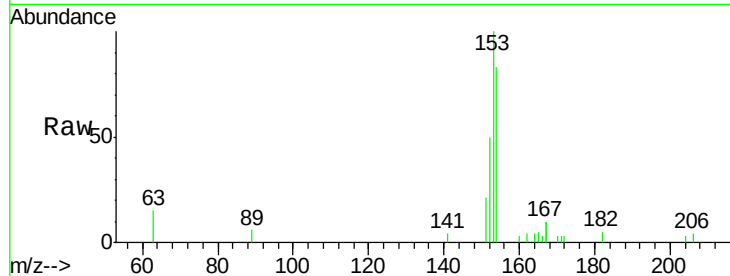


Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E

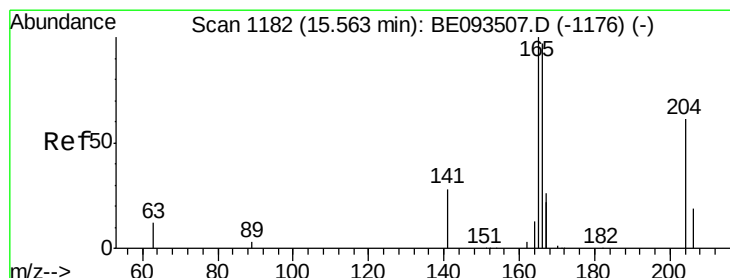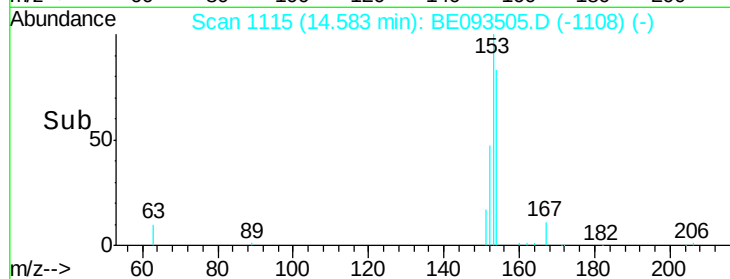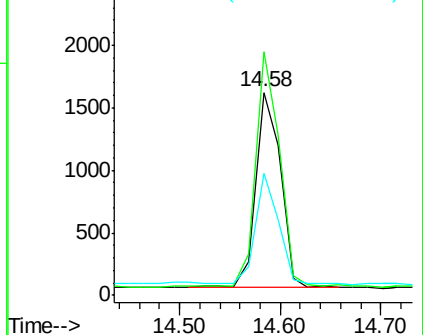

#18
Fluorene
Concen: 0.116 ng
RT: 15.58 min Scan# 1182
Delta R.T. 0.01 min
Lab File: BE093505.D
Acq: 21 Jul 2017 12:31

Tgt Ion:166 Resp: 3817
Ion Ratio Lower Upper
166 100
165 99.1 78.6 117.8
167 54.6 11.1 16.7#

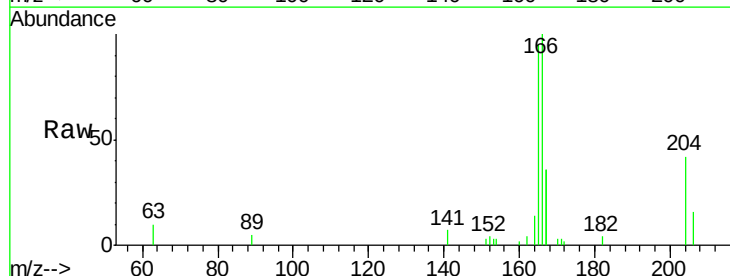

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

