
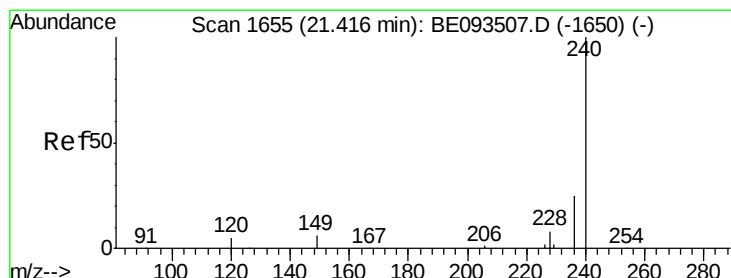
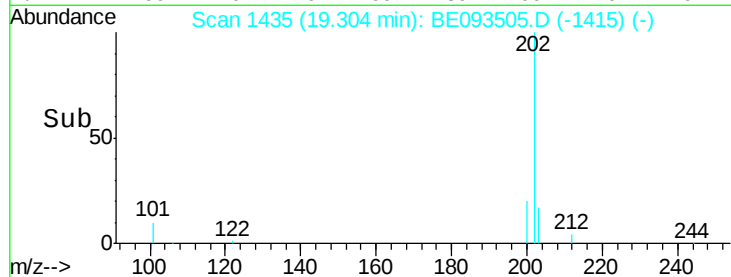
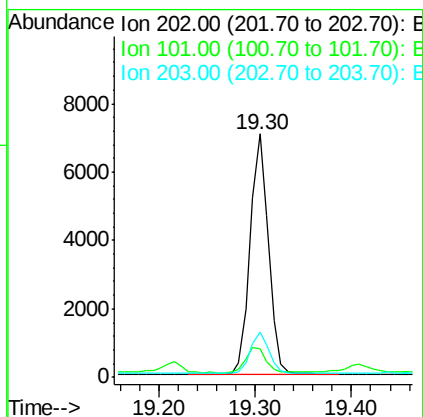


#26
 Fluoranthene
 Concen: 0.156 ng
 RT: 19.30 min Scan# 1435
 Delta R.T. 0.00 min
 Lab File: BE093505.D
 Acq: 21 Jul 2017 12:31

Instrument :
 BNA_E
 ClientSampleId :

Tgt Ion:202 Resp: 9460
 Ion Ratio Lower Upper
 202 100
 101 11.3 9.6 14.4
 203 17.1 14.4 21.6

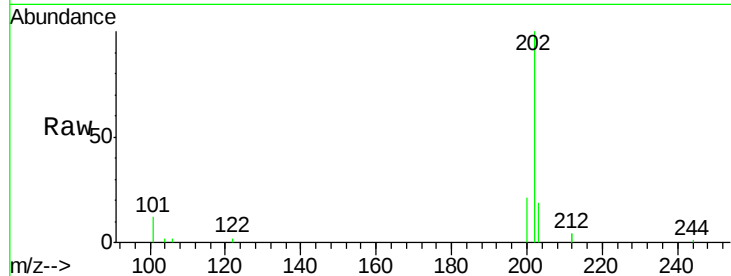

#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.42 min Scan# 1654
 Delta R.T. 0.00 min
 Lab File: BE093505.D
 Acq: 21 Jul 2017 12:31

Tgt Ion:240 Resp: 32157
 Ion Ratio Lower Upper
 240 100
 120 5.9 4.6 7.0
 236 25.0 20.8 31.2

