

#30

Benzo(a)anthracene

Concen: 0.120 ng

RT: 21.39 min Scan# 1652

Delta R.T. 0.00 min

Lab File: BE093505.D

Acq: 21 Jul 2017 12:31

Instrument :

BNA_E

ClientSampled :


Tgt Ion:228 Resp: 10447

Ion Ratio Lower Upper

228 100

226 27.1 19.7 29.5




229 21.4 19.2 28.8

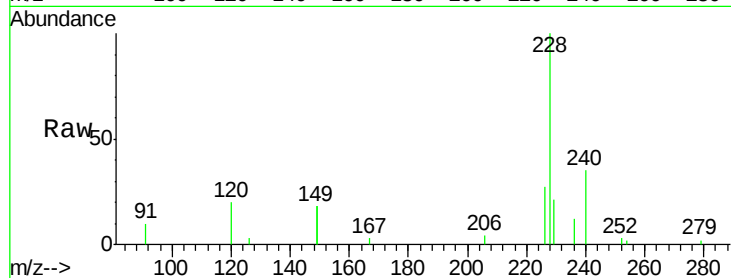

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

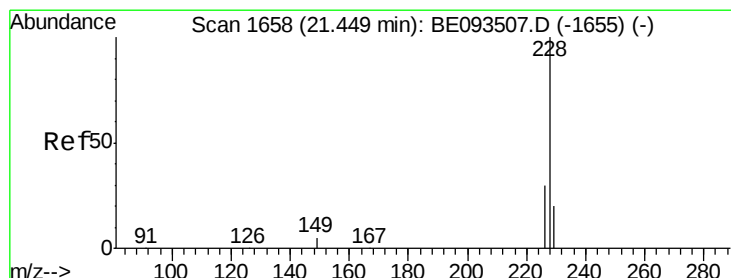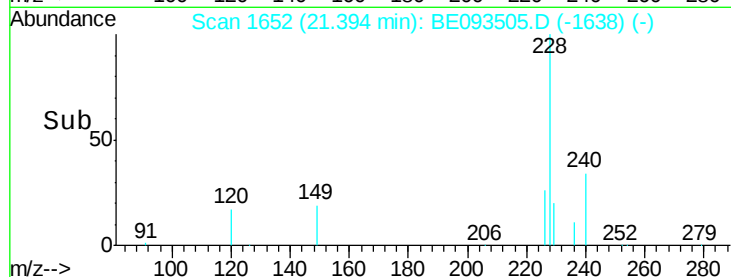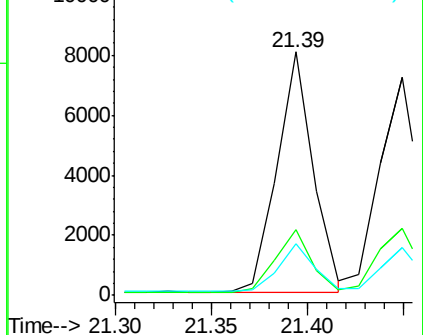

#31

Chrysene

Concen: 0.114 ng

RT: 21.45 min Scan# 1657

Delta R.T. 0.00 min

Lab File: BE093505.D

Acq: 21 Jul 2017 12:31


Tgt Ion:228 Resp: 10359

Ion Ratio Lower Upper

228 100

226 30.6 21.5 32.3

229 21.8 18.6 28.0

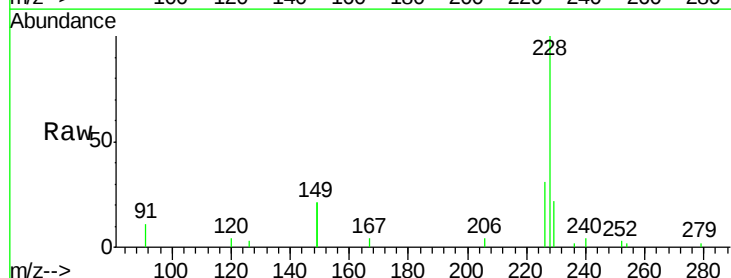

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

