
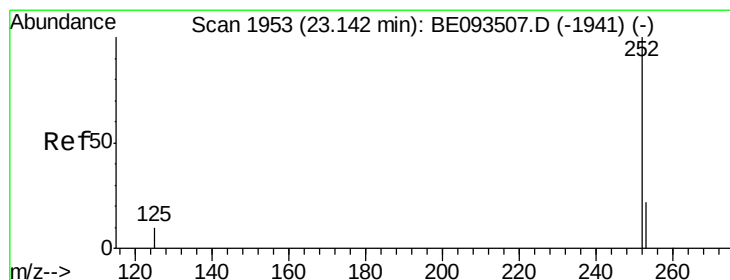
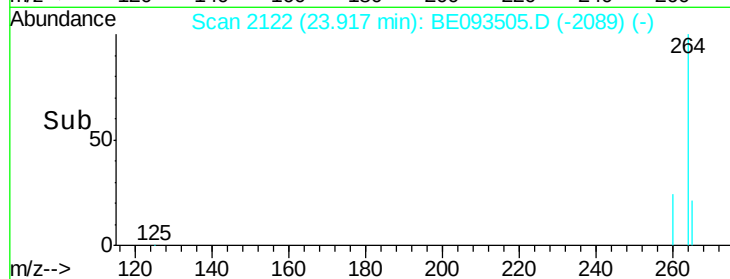
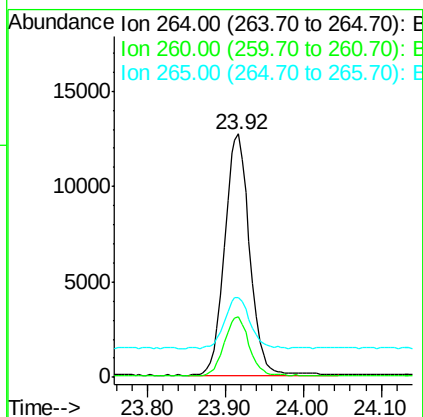


#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.92 min Scan# 2122
 Delta R.T. 0.00 min
 Lab File: BE093505.D
 Acq: 21 Jul 2017 12:31

Instrument :
 BNA_E
 ClientSampleId :

Tgt Ion: 264 Resp: 28135
 Ion Ratio Lower Upper
 264 100
 260 24.7 21.0 31.4
 265 32.6 24.6 36.8

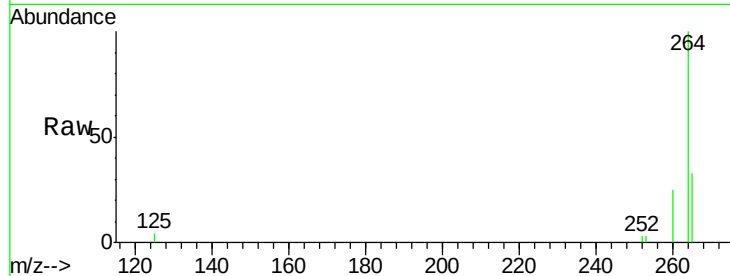

#35
 Benzo(b)fluoranthene
 Concen: 0.106 ng
 RT: 23.14 min Scan# 1952
 Delta R.T. 0.00 min
 Lab File: BE093505.D
 Acq: 21 Jul 2017 12:31

Tgt Ion: 252 Resp: 9615
 Ion Ratio Lower Upper
 252 100
 253 29.6 18.5 27.7#
 125 20.3 13.4 20.0#

