
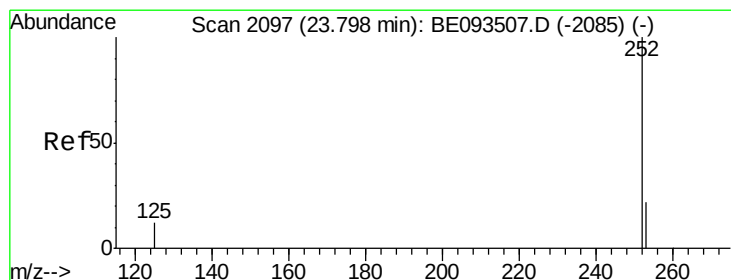
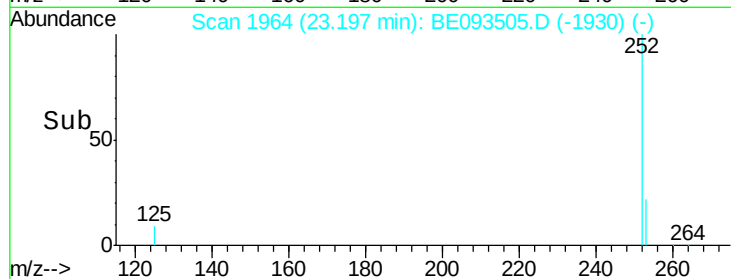
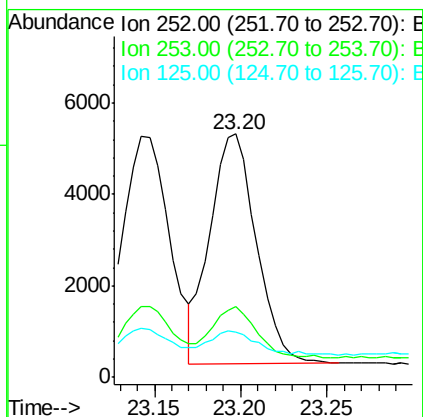


#36
Benzo(k)fluoranthene
Concen: 0.105 ng
RT: 23.20 min Scan# 1964
Delta R.T. 0.00 min
Lab File: BE093505.D
Acq: 21 Jul 2017 12:31

Instrument :
BNA_E
ClientSampleId :

Tgt Ion: 252 Resp: 9435
Ion Ratio Lower Upper
252 100
253 29.1 20.3 30.5
125 18.8 12.2 18.4#

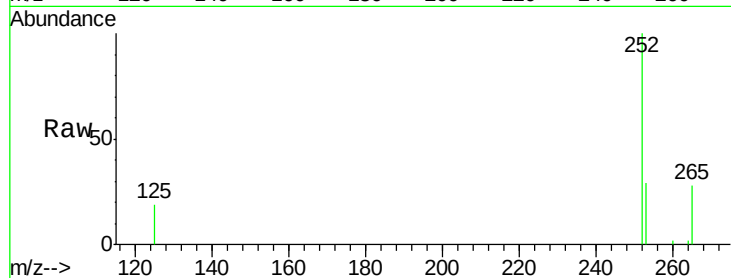

#37
Benzo(a)pyrene
Concen: 0.115 ng
RT: 23.80 min Scan# 2097
Delta R.T. 0.00 min
Lab File: BE093505.D
Acq: 21 Jul 2017 12:31

Tgt Ion: 252 Resp: 9192
Ion Ratio Lower Upper
252 100
253 30.1 19.9 29.9#
125 22.7 14.6 21.8#

