

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.71 min Scan# 577

Delta R.T. -0.00 min

Lab File: BE093506.D


Acq: 21 Jul 2017 13:07

Instrument :

BNA_E

ClientSampleId :

Tgt Ion:	136	Resp:	13768
Ion Ratio	Lower	Upper	
136	100		
137	11.5	9.8	14.8
54	49.9	10.3	15.5#
68	9.8	9.0	13.4



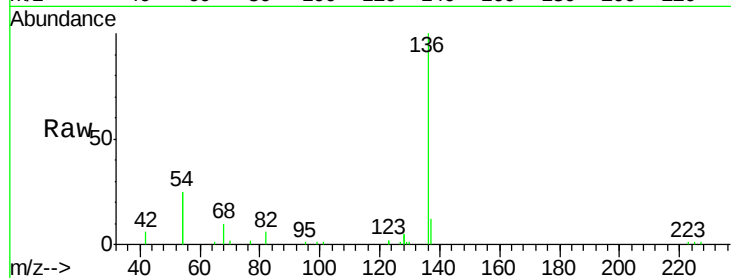


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

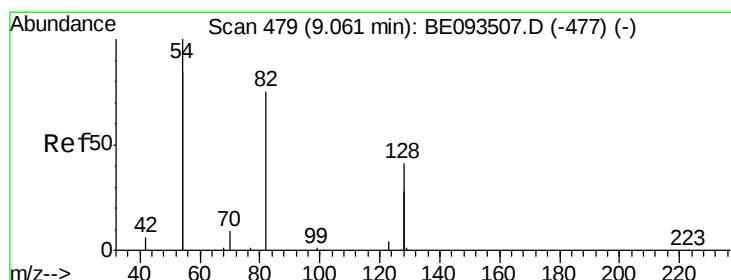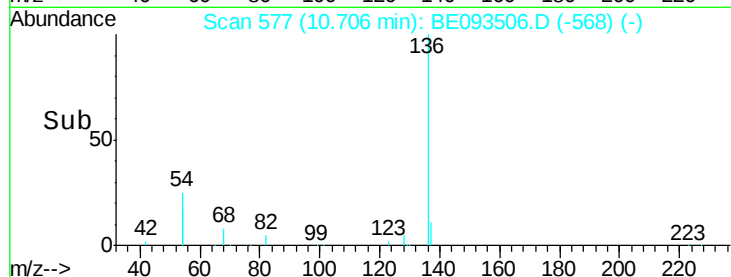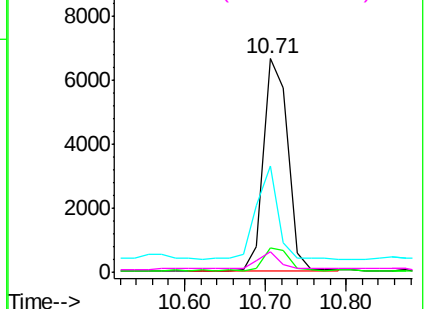

#8

Nitrobenzene-d5

Concen: 0.262 ng


RT: 9.06 min Scan# 479

Delta R.T. -0.00 min

Lab File: BE093506.D

Acq: 21 Jul 2017 13:07

Tgt Ion:	82	Resp:	2300
Ion Ratio	Lower	Upper	
82	100		
128	111.0	17.0	25.4#
54	263.4	53.8	80.6#

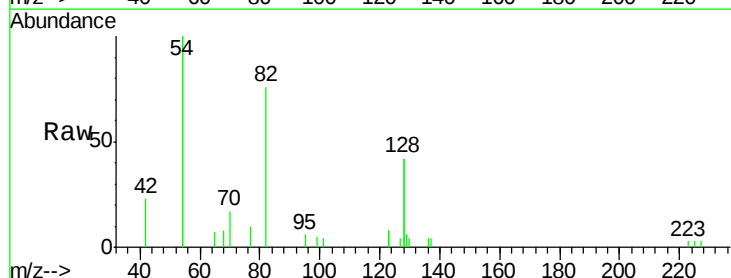

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

