
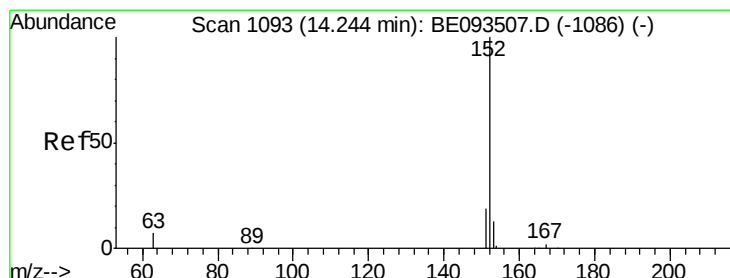
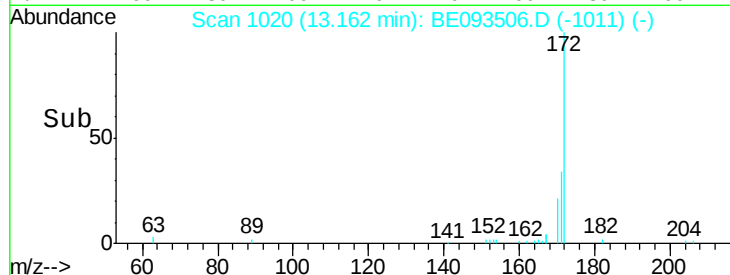
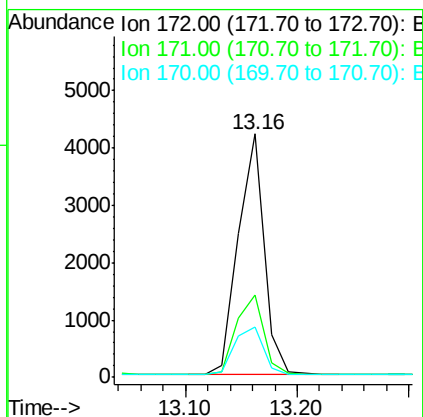


#15
2-Fluorobiphenyl
Concen: 0.207 ng
RT: 13.16 min Scan# 1020
Delta R.T. -0.00 min
Lab File: BE093506.D
Acq: 21 Jul 2017 13:07

Instrument :
BNA_E
ClientSampled :

Tgt Ion:172 Resp: 6739
Ion Ratio Lower Upper
172 100
171 33.6 29.8 44.6
170 20.9 20.7 31.1

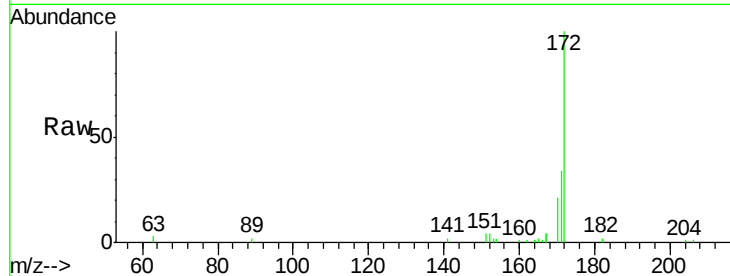

#16
Acenaphthylene
Concen: 0.241 ng
RT: 14.24 min Scan# 1093
Delta R.T. -0.00 min
Lab File: BE093506.D
Acq: 21 Jul 2017 13:07

Tgt Ion:152 Resp: 8432
Ion Ratio Lower Upper
152 100
151 20.5 4.0 6.0#
153 13.3 10.3 15.5

