

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.24 min Scan# 1243

Delta R.T. -0.00 min

Lab File: BE093506.D

Acq: 21 Jul 2017 13:07

Instrument :

BNA_E

ClientSampleId :


Tgt Ion:188 Resp: 20303

Ion Ratio Lower Upper

188 100

94 20.8 11.3 16.9#




80 22.2 11.7 17.5#

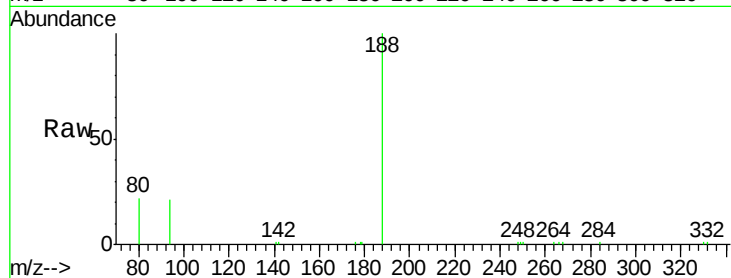

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

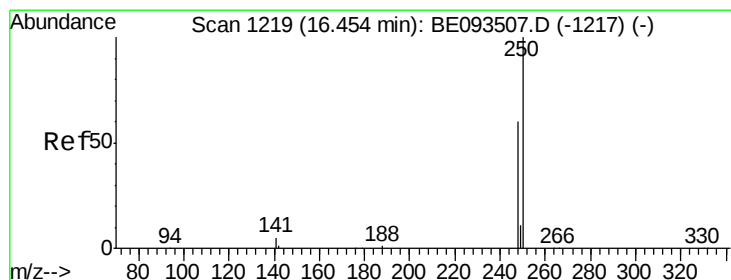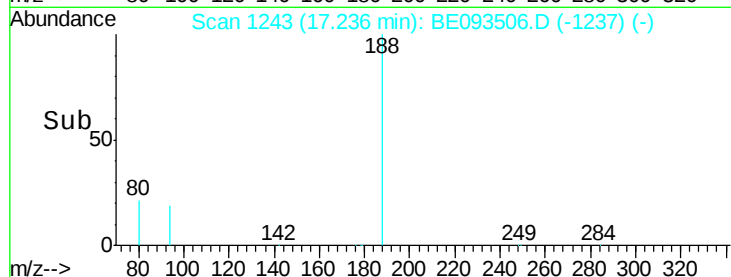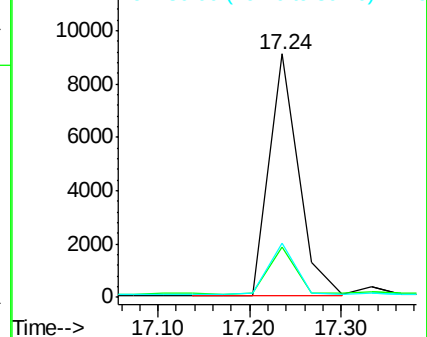

#20

4-Bromophenyl-phenylether

Concen: 0.158 ng

RT: 16.45 min Scan# 1219

Delta R.T. 0.00 min

Lab File: BE093506.D

Acq: 21 Jul 2017 13:07


Tgt Ion:248 Resp: 1760

Ion Ratio Lower Upper

248 100

250 152.5 128.0 192.0

141 19.1 12.0 18.0#

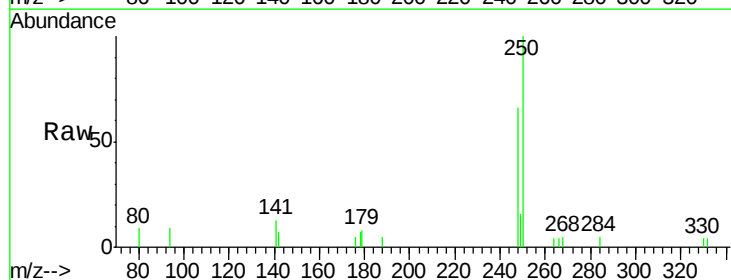

Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

