

#24

Anthracene

Concen: 0.535 ng

RT: 17.37 min Scan# 1247

Delta R.T. -0.00 min

Lab File: BE093506.D

Acq: 21 Jul 2017 13:07

Instrument :

BNA_E

ClientSampleId :





Tgt Ion:178 Resp: 24223

Ion Ratio Lower Upper

178 100

176 19.7 14.6 22.0

179 7.8 12.0 18.0#

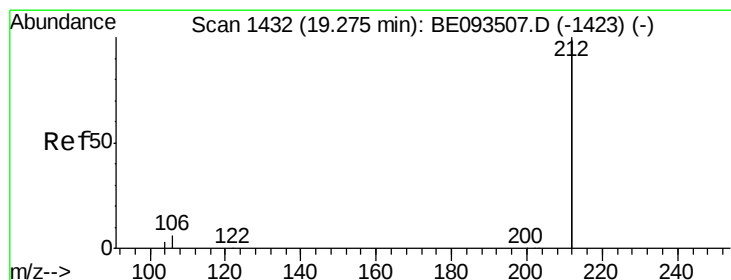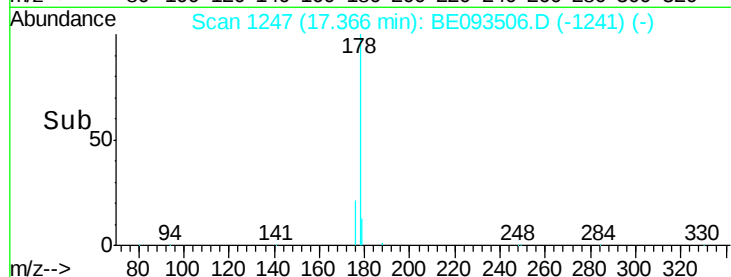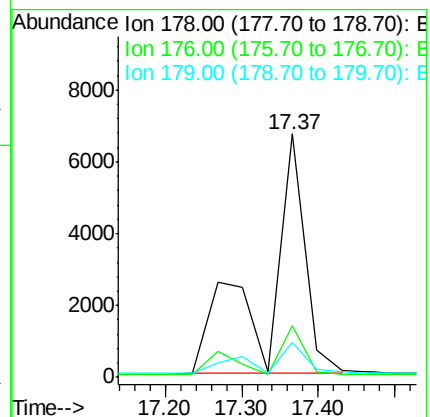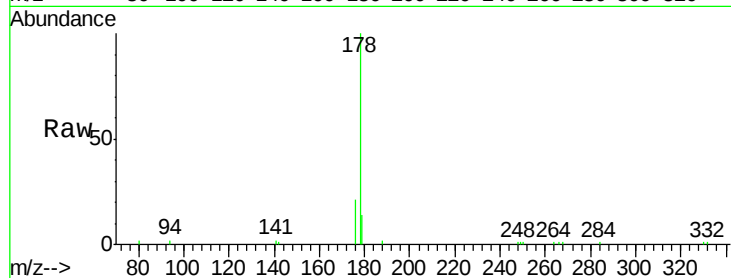

#25

Fluoranthene-d10

Concen: 0.268 ng

RT: 19.27 min Scan# 1432

Delta R.T. -0.00 min

Lab File: BE093506.D

Acq: 21 Jul 2017 13:07

Tgt Ion:212 Resp: 65526

Ion Ratio Lower Upper

212 100

106 3.2 2.4 3.6

104 1.9 1.6 2.4

