
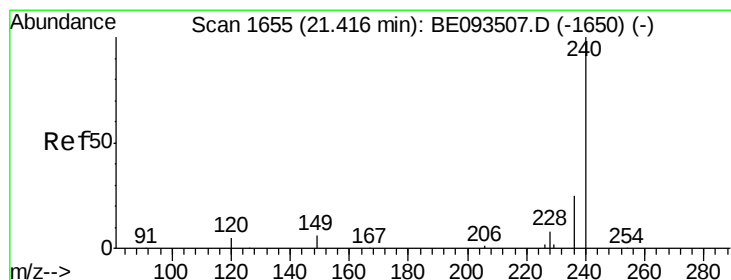
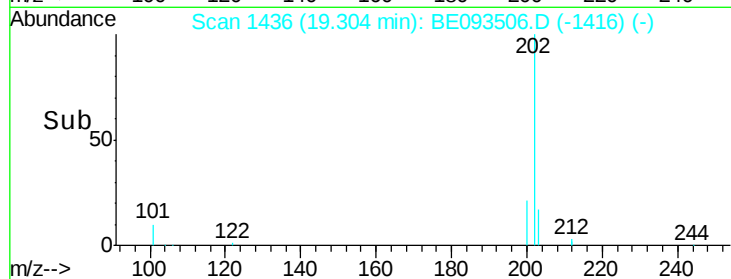
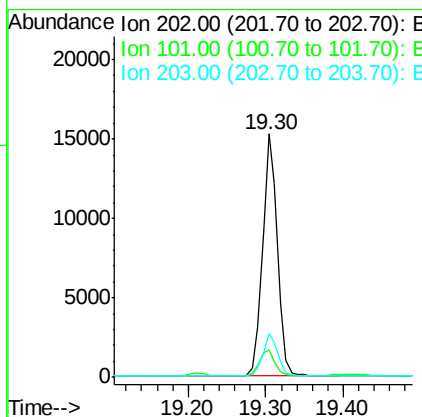


#26  
 Fluoranthene  
 Concen: 0.299 ng  
 RT: 19.30 min Scan# 1436  
 Delta R.T. -0.00 min  
 Lab File: BE093506.D  
 Acq: 21 Jul 2017 13:07

Instrument :  
 BNA\_E  
 ClientSampleId :

Tgt Ion:202 Resp: 20709  
 Ion Ratio Lower Upper  
 202 100  
 101 10.8 9.6 14.4  
 203 17.2 14.4 21.6

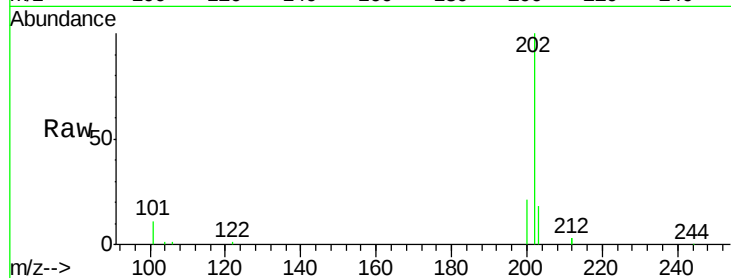

#27  
 Chrysene-d12  
 Concen: 0.400 ng  
 RT: 21.42 min Scan# 1655  
 Delta R.T. -0.00 min  
 Lab File: BE093506.D  
 Acq: 21 Jul 2017 13:07

Tgt Ion:240 Resp: 31784  
 Ion Ratio Lower Upper  
 240 100  
 120 6.7 4.6 7.0  
 236 26.1 20.8 31.2

