
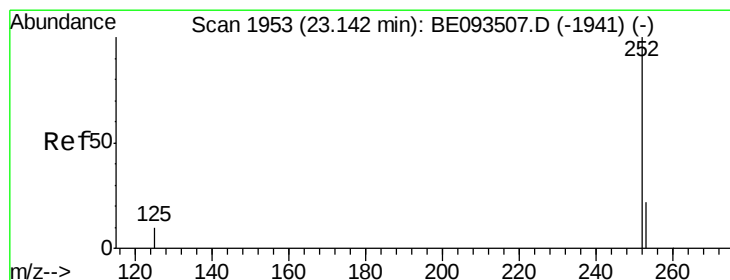
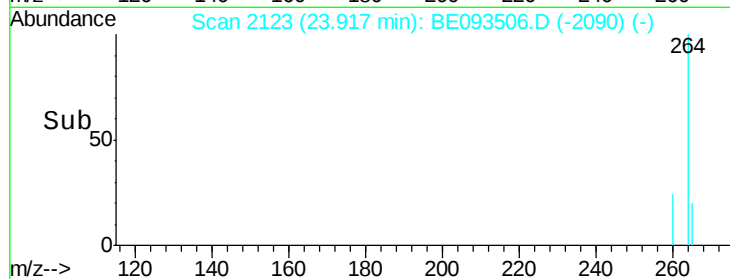
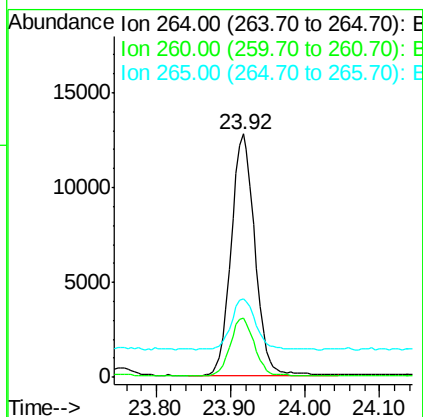


#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.92 min Scan# 2123
 Delta R.T. -0.00 min
 Lab File: BE093506.D
 Acq: 21 Jul 2017 13:07

Instrument :
 BNA_E
 ClientSampleId :

Tgt Ion:264 Resp: 28067
 Ion Ratio Lower Upper
 264 100
 260 24.3 21.0 31.4
 265 32.0 24.6 36.8

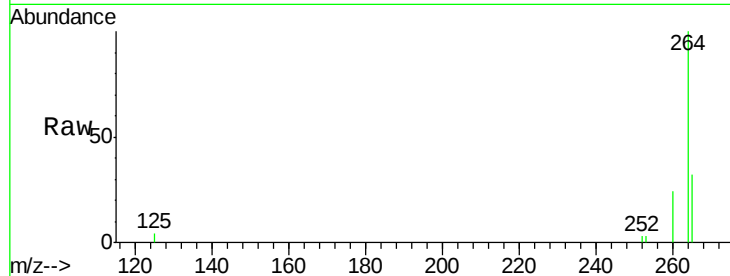

#35
 Benzo(b)fluoranthene
 Concen: 0.219 ng
 RT: 23.15 min Scan# 1954
 Delta R.T. 0.00 min
 Lab File: BE093506.D
 Acq: 21 Jul 2017 13:07

Tgt Ion:252 Resp: 19889
 Ion Ratio Lower Upper
 252 100
 253 25.1 18.5 27.7
 125 14.9 13.4 20.0

