

#36

Benzo(k)fluoranthene

Concen: 0.221 ng

RT: 23.20 min Scan# 1965

Delta R.T. 0.00 min

Lab File: BE093506.D

Acq: 21 Jul 2017 13:07

Instrument :

BNA_E

ClientSampleId :





Tgt Ion: 252 Resp: 19836

Ion Ratio Lower Upper

252 100

253 24.9 20.3 30.5

125 13.6 12.2 18.4

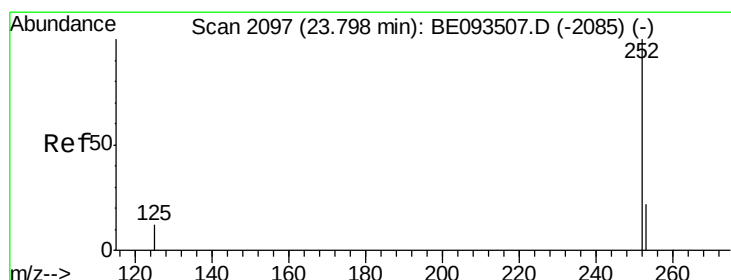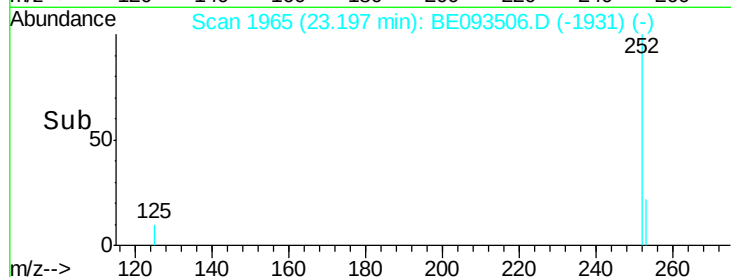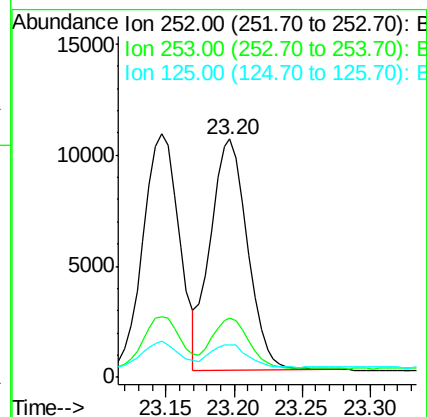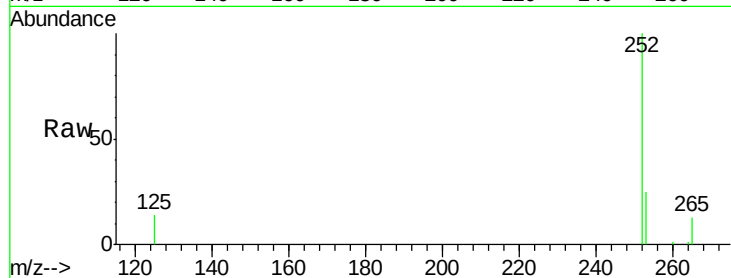

#37

Benzo(a)pyrene

Concen: 0.234 ng

RT: 23.80 min Scan# 2098

Delta R.T. 0.00 min

Lab File: BE093506.D

Acq: 21 Jul 2017 13:07

Tgt Ion: 252 Resp: 18606

Ion Ratio Lower Upper

252 100

253 25.6 19.9 29.9

125 16.7 14.6 21.8

