

#38

Dibenzo(a,h)anthracene

Concen: 0.227 ng

RT: 26.58 min Scan# 2705

Delta R.T. 0.01 min


Lab File: BE093506.D

Acq: 21 Jul 2017 13:07

Instrument :

BNA_E

ClientSampleId :

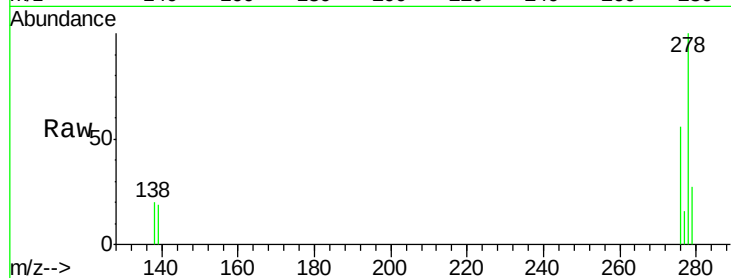




Tgt Ion:278 Resp: 17485

Ion Ratio Lower Upper

278 100

139 19.0 21.4 32.0#

279 26.6 22.2 33.2

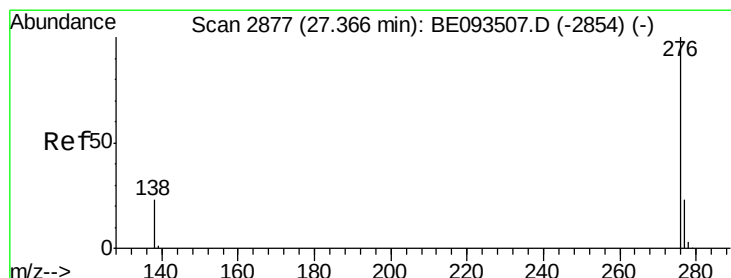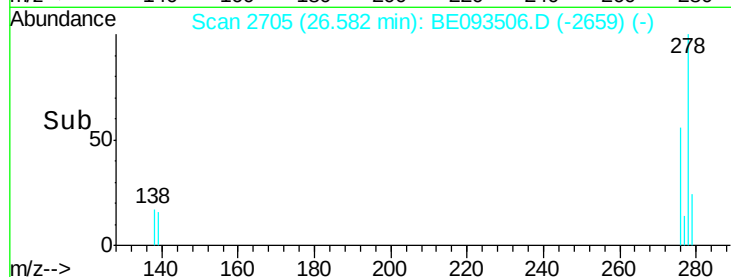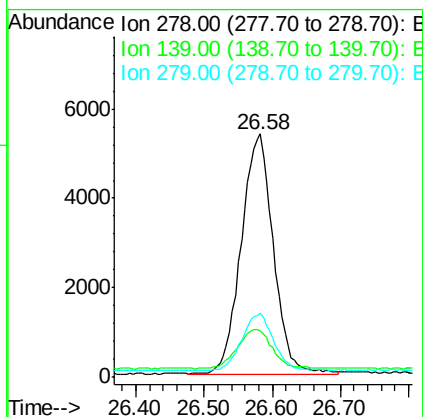

#39

Benzo(g,h,i)perylene

Concen: 0.227 ng

RT: 27.37 min Scan# 2877

Delta R.T. 0.00 min

Lab File: BE093506.D

Acq: 21 Jul 2017 13:07

Tgt Ion:276 Resp: 17677

Ion Ratio Lower Upper

276 100

277 25.3 21.2 31.8

138 24.7 24.5 36.7

