


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.93 min Scan# 403
Delta R.T. 0.00 min
Lab File: BE093507.D
Acq: 21 Jul 2017 13:43

Instrument :
BNA_E
ClientSampleId :

Tgt Ion: 152 Resp: 2748
Ion Ratio Lower Upper
152 100
150 152.8 125.1 187.7
115 67.6 55.7 83.5

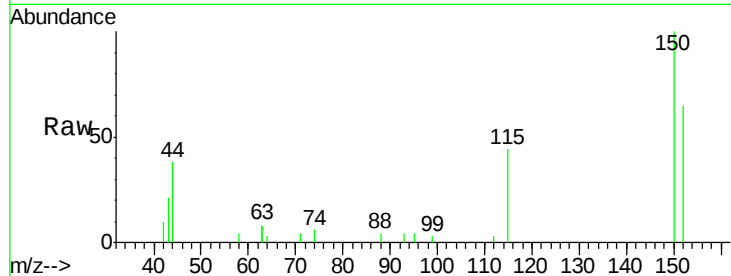


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

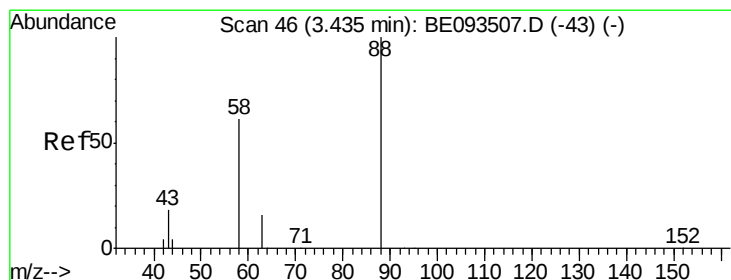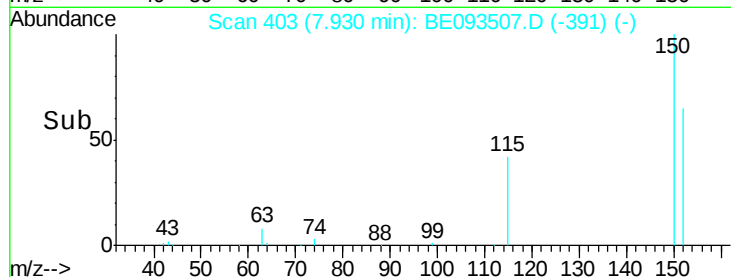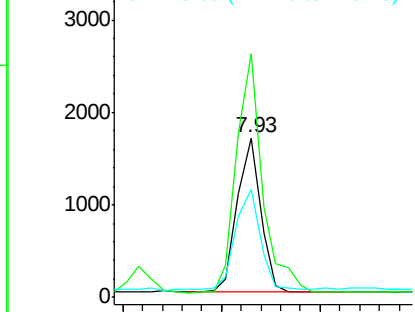

#2

1,4-Dioxane
Concen: 0.311 ng
RT: 3.44 min Scan# 46
Delta R.T. 0.00 min
Lab File: BE093507.D
Acq: 21 Jul 2017 13:43

Tgt Ion: 88 Resp: 1809
Ion Ratio Lower Upper
88 100
58 77.6 62.2 93.4
43 34.9 23.2 34.8#

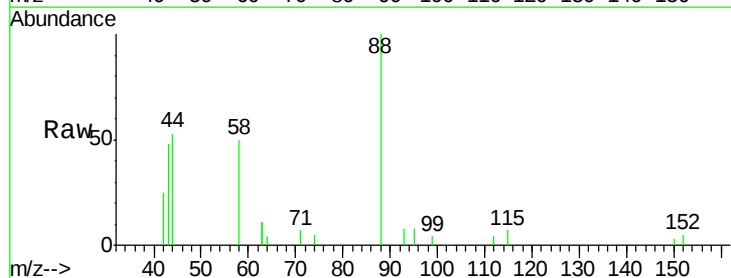

Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

