

#3

n-Nitrosodimethylamine

Concen: 0.551 ng

RT: 3.74 min Scan# 70

Delta R.T. 0.00 min

Lab File: BE093507.D

Acq: 21 Jul 2017 13:43

Instrument :

BNA\_E

ClientSampleId :


Tgt Ion: 42 Resp: 1681

Ion Ratio Lower Upper




42 100

74 146.9 99.1 148.7

44 11.3 7.4 11.2#

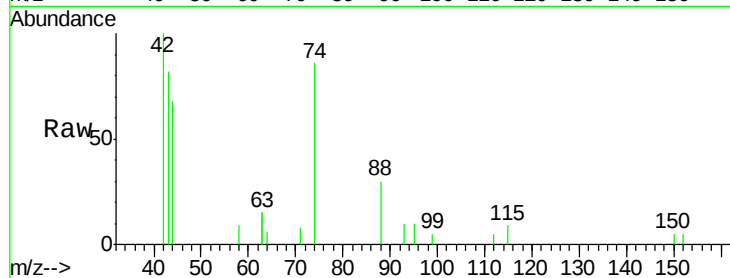

Abundance Ion 42.00 (41.70 to 42.70): BE0  
Ion 74.00 (73.70 to 74.70): BE0  
Ion 44.00 (43.70 to 44.70): BE0

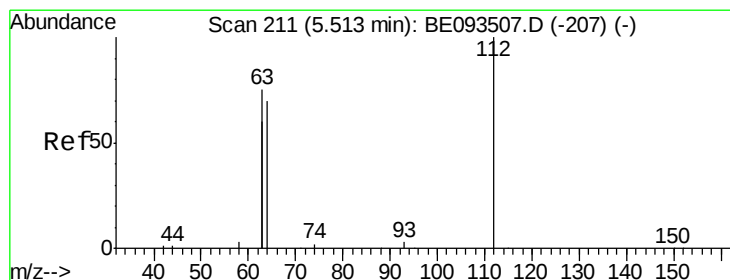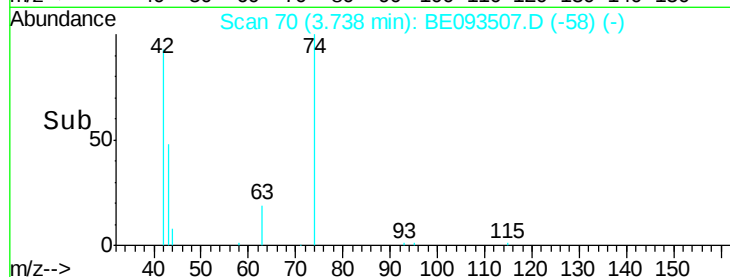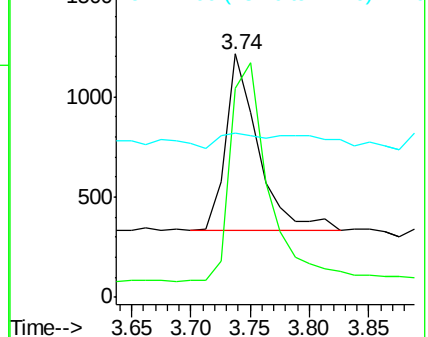

#4

2-Fluorophenol

Concen: 0.456 ng

RT: 5.51 min Scan# 211

Delta R.T. 0.00 min

Lab File: BE093507.D

Acq: 21 Jul 2017 13:43


Tgt Ion: 112 Resp: 3783

Ion Ratio Lower Upper

112 100

64 66.8 56.4 84.6

63 133.4 29.3 43.9#

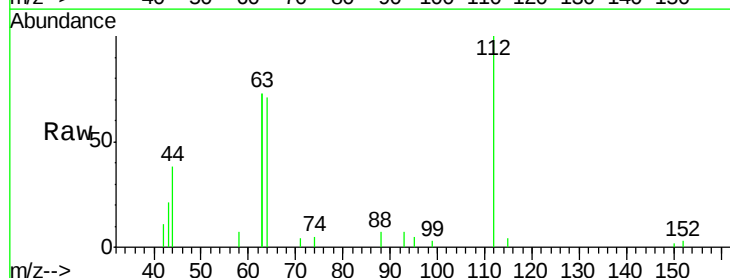

Abundance Ion 112.00 (111.70 to 112.70): E  
Ion 64.00 (63.70 to 64.70): BE0  
Ion 63.00 (62.70 to 63.70): BE0

