

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.71 min Scan# 577

Delta R.T. 0.00 min

Lab File: BE093507.D

Acq: 21 Jul 2017 13:43

Instrument :

BNA_E

ClientSampleId :

Tgt Ion: 136 Resp: 13376


Ion Ratio Lower Upper

136 100

137 11.3 9.8 14.8

54 48.1 10.3 15.5#

68 10.3 9.0 13.4



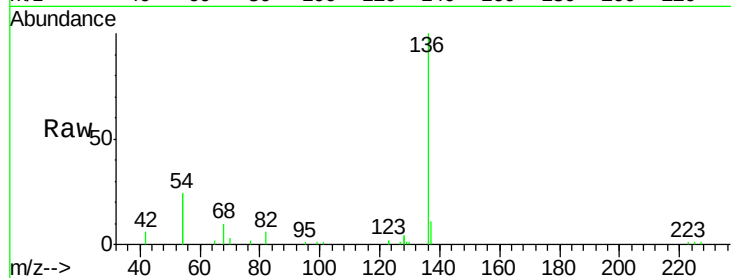


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

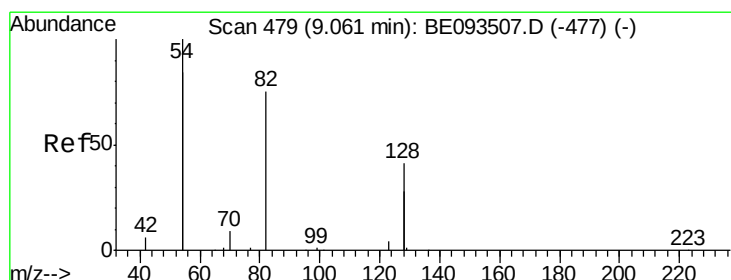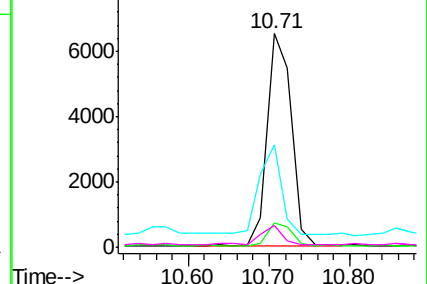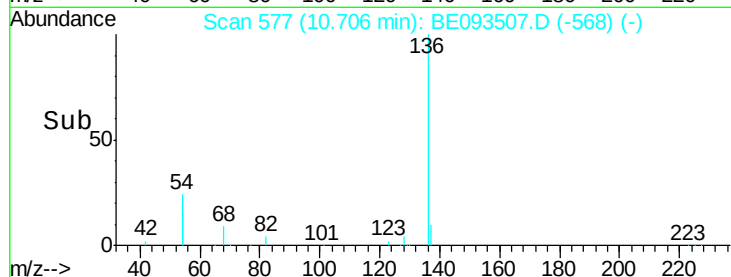

#8

Nitrobenzene-d5

Concen: 0.475 ng

RT: 9.06 min Scan# 479

Delta R.T. 0.00 min

Lab File: BE093507.D

Acq: 21 Jul 2017 13:43


Tgt Ion: 82 Resp: 4055

Ion Ratio Lower Upper

82 100

128 104.5 17.0 25.4#

54 256.5 53.8 80.6#

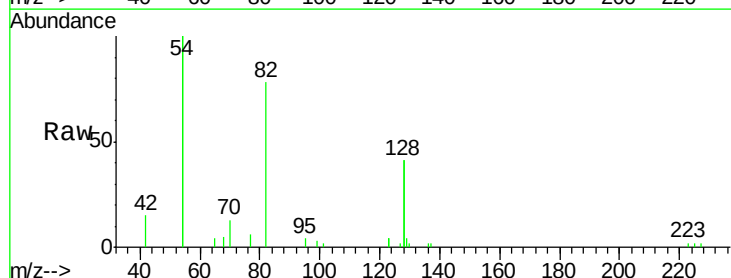

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

