
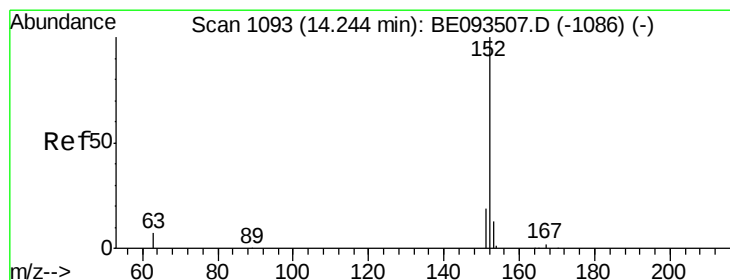
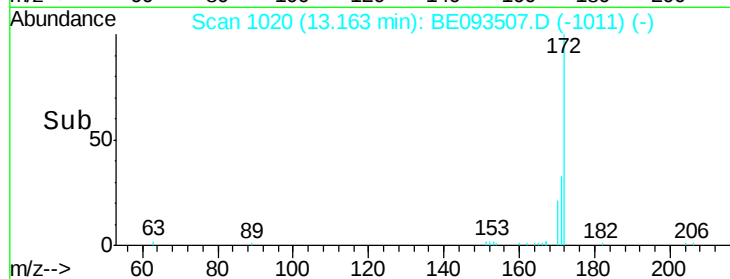
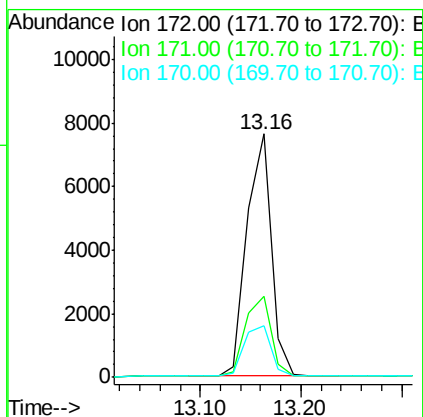


#15
2-Fluorobiphenyl
Concen: 0.417 ng
RT: 13.16 min Scan# 1020
Delta R.T. 0.00 min
Lab File: BE093507.D
Acq: 21 Jul 2017 13:43

Instrument :
BNA_E
ClientSampleId :

Tgt Ion:172 Resp: 12884
Ion Ratio Lower Upper
172 100
171 33.2 29.8 44.6
170 21.2 20.7 31.1

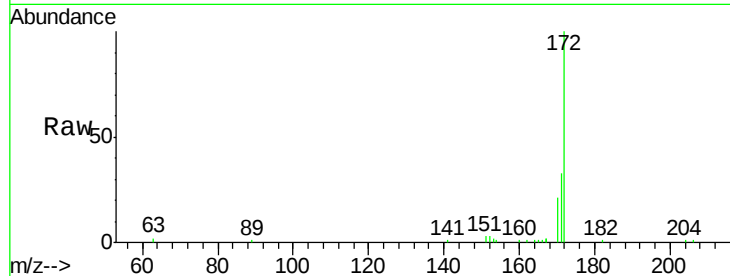

#16
Acenaphthylene
Concen: 0.468 ng
RT: 14.24 min Scan# 1093
Delta R.T. 0.00 min
Lab File: BE093507.D
Acq: 21 Jul 2017 13:43

Tgt Ion:152 Resp: 15517
Ion Ratio Lower Upper
152 100
151 19.1 4.0 6.0#
153 13.1 10.3 15.5

