

#24

Anthracene

Concen: 0.972 ng

RT: 17.37 min Scan# 1247

Delta R.T. 0.00 min

Lab File: BE093507.D

Acq: 21 Jul 2017 13:43

Instrument :

BNA_E

ClientSampleId :





Tgt Ion:178 Resp: 45894

Ion Ratio Lower Upper

178 100

176 20.4 14.6 22.0

179 14.3 12.0 18.0

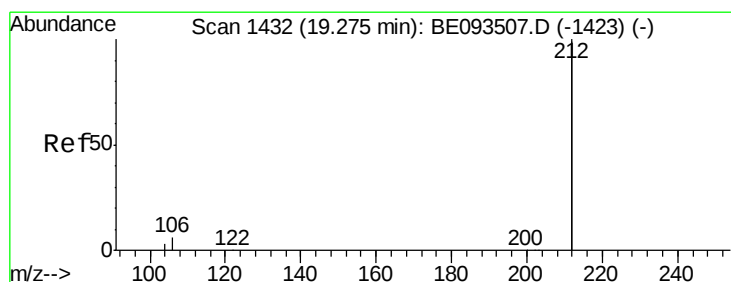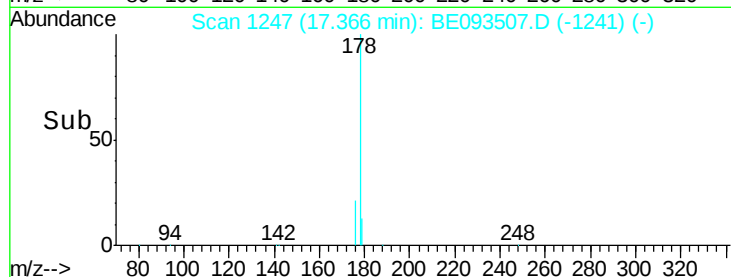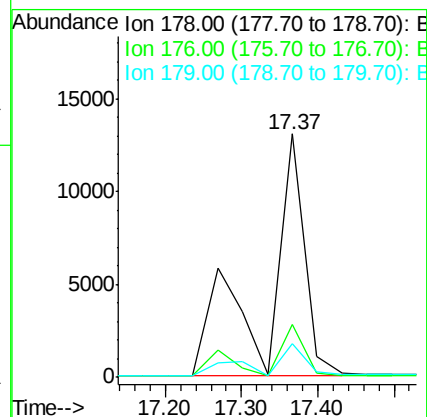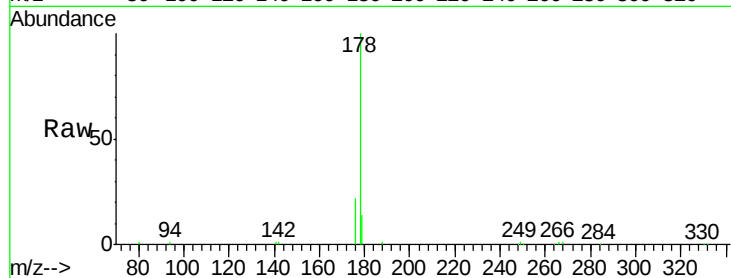

#25

Fluoranthene-d10

Concen: 0.510 ng

RT: 19.27 min Scan# 1432

Delta R.T. 0.00 min

Lab File: BE093507.D

Acq: 21 Jul 2017 13:43

Tgt Ion:212 Resp: 130271

Ion Ratio Lower Upper

212 100

106 3.2 2.4 3.6

104 1.8 1.6 2.4

