
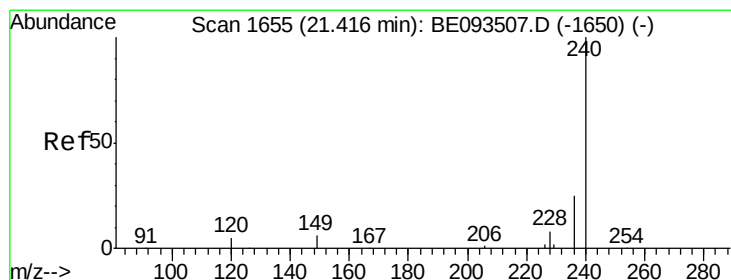
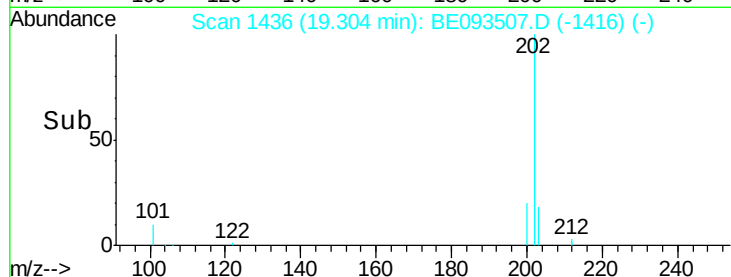
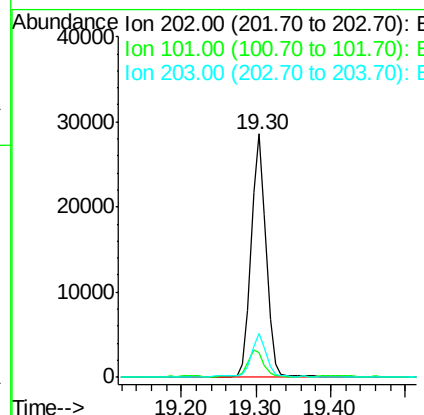


#26
 Fluoranthene
 Concen: 0.540 ng
 RT: 19.30 min Scan# 1436
 Delta R.T. 0.00 min
 Lab File: BE093507.D
 Acq: 21 Jul 2017 13:43

Instrument :
 BNA_E
 ClientSampleId :

Tgt Ion: 202 Resp: 39071
 Ion Ratio Lower Upper
 202 100
 101 11.2 9.6 14.4
 203 17.3 14.4 21.6

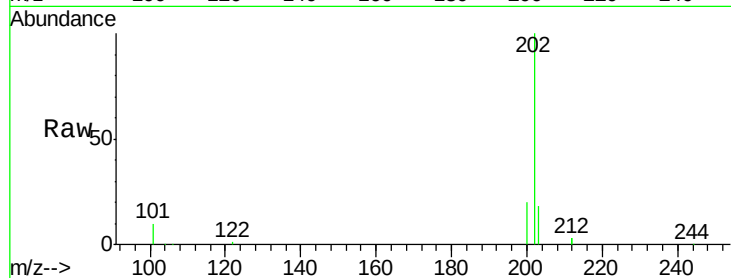

#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.42 min Scan# 1655
 Delta R.T. 0.00 min
 Lab File: BE093507.D
 Acq: 21 Jul 2017 13:43

Tgt Ion: 240 Resp: 31626
 Ion Ratio Lower Upper
 240 100
 120 6.6 4.6 7.0
 236 25.9 20.8 31.2

