

#30

Benzo(a)anthracene

Concen: 0.469 ng

RT: 21.39 min Scan# 1653

Delta R.T. 0.00 min

Lab File: BE093507.D





Acq: 21 Jul 2017 13:43

Instrument :

BNA_E

ClientSampleId :

Tgt Ion:	228	Resp:	40005
Ion	Ratio	Lower	Upper
228	100		
226	26.1	19.7	29.5
229	19.8	19.2	28.8

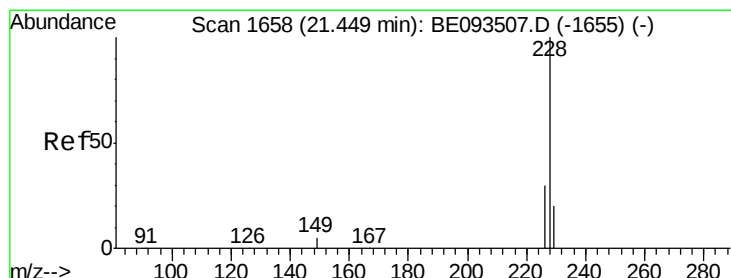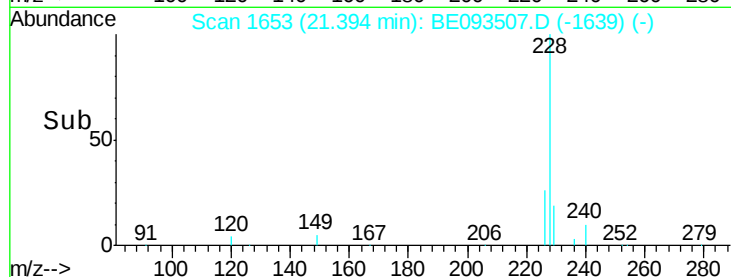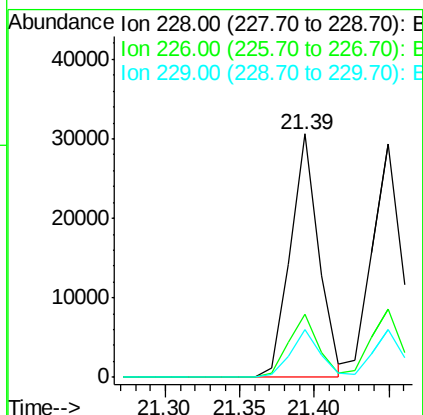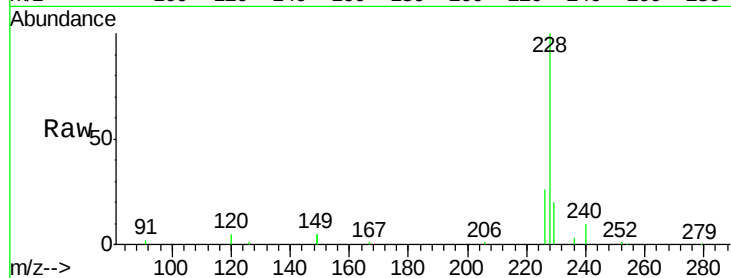

#31

Chrysene

Concen: 0.452 ng

RT: 21.45 min Scan# 1658

Delta R.T. 0.00 min

Lab File: BE093507.D

Acq: 21 Jul 2017 13:43

Tgt Ion:	228	Resp:	40395
Ion	Ratio	Lower	Upper
228	100		
226	29.4	21.5	32.3
229	20.2	18.6	28.0

