

#36

Benzo(k)fluoranthene

Concen: 0.428 ng

RT: 23.19 min Scan# 1964

Delta R.T. 0.00 min

Lab File: BE093507.D

Acq: 21 Jul 2017 13:43





Instrument :

BNA_E

ClientSampleId :

Tgt Ion:252 Resp: 36401

Ion	Ratio	Lower	Upper
252	100		
253	23.6	20.3	30.5
125	12.1	12.2	18.4#

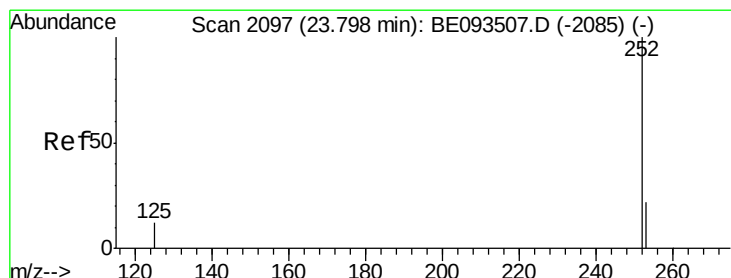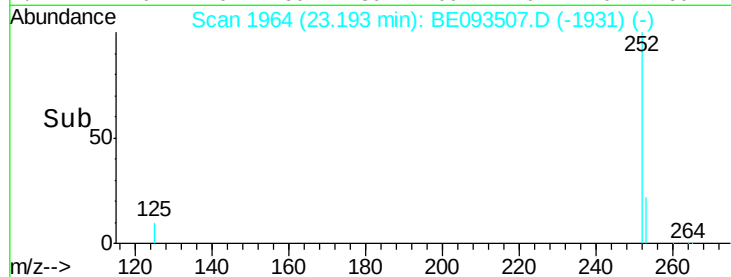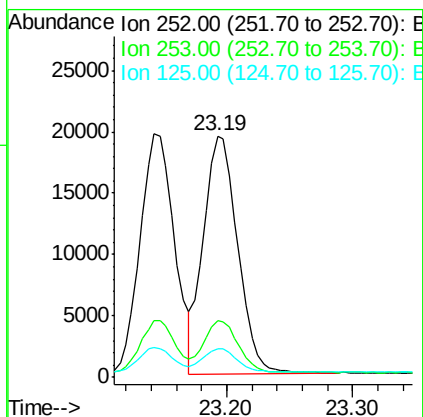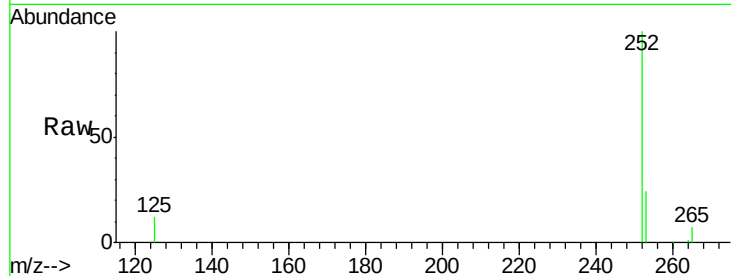

#37

Benzo(a)pyrene

Concen: 0.450 ng

RT: 23.80 min Scan# 2097

Delta R.T. 0.00 min

Lab File: BE093507.D

Acq: 21 Jul 2017 13:43

Tgt Ion:252 Resp: 33965

Ion	Ratio	Lower	Upper
252	100		
253	23.9	19.9	29.9
125	13.9	14.6	21.8#

