
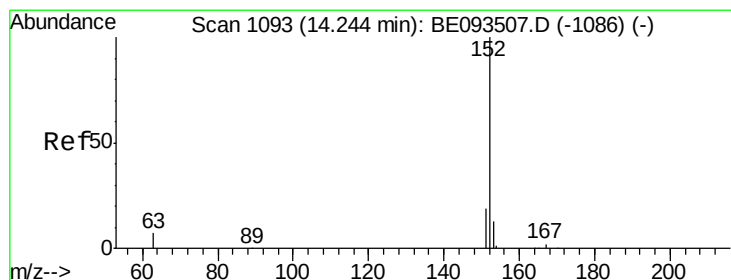
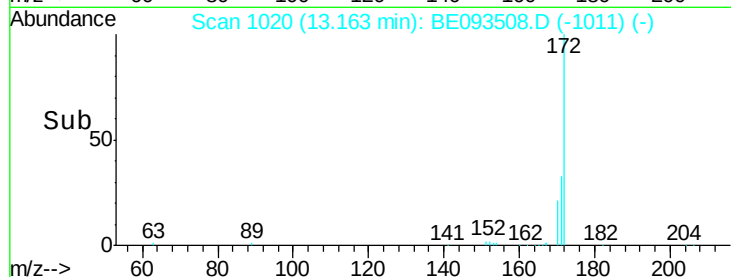
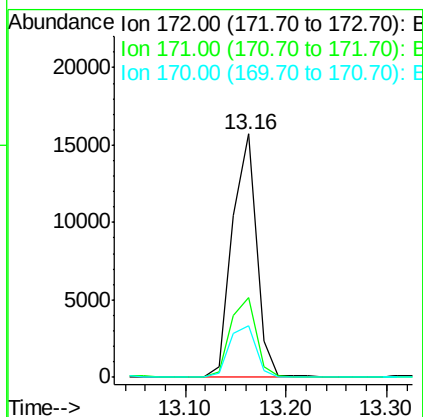


#15
2-Fluorobiphenyl
Concen: 0.796 ng
RT: 13.16 min Scan# 1020
Delta R.T. -0.00 min
Lab File: BE093508.D
Acq: 21 Jul 2017 14:21

Instrument :
BNA_E
ClientSampleId :

Tgt Ion:172 Resp: 25950
Ion Ratio Lower Upper
172 100
171 32.9 29.8 44.6
170 21.0 20.7 31.1

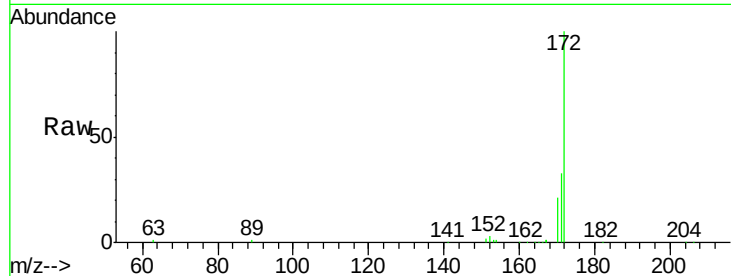

#16
Acenaphthylene
Concen: 0.955 ng
RT: 14.24 min Scan# 1093
Delta R.T. -0.00 min
Lab File: BE093508.D
Acq: 21 Jul 2017 14:21

Tgt Ion:152 Resp: 33408
Ion Ratio Lower Upper
152 100
151 19.3 4.0 6.0#
153 13.0 10.3 15.5

