

#24

Anthracene

Concen: 2.013 ng

RT: 17.37 min Scan# 1247

Delta R.T. -0.00 min

Lab File: BE093508.D

Acq: 21 Jul 2017 14:21

Instrument :

BNA_E

ClientSampleId :





Tgt Ion:178 Resp: 93364

Ion Ratio Lower Upper

178 100

176 20.7 14.6 22.0

179 8.1 12.0 18.0#

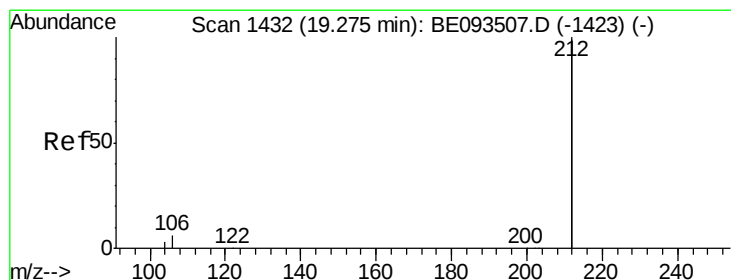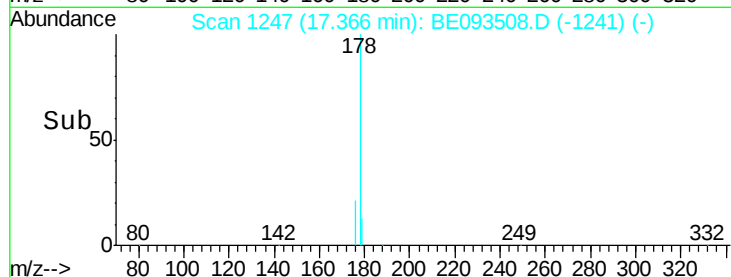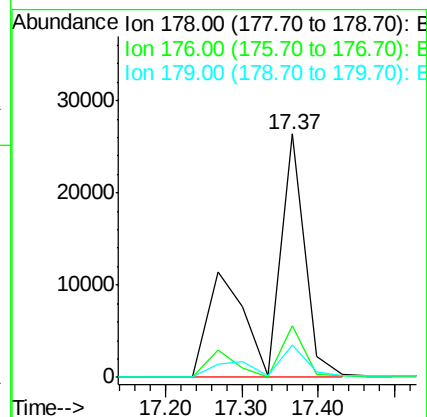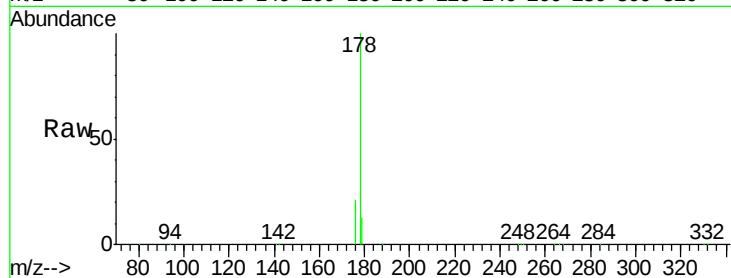

#25

Fluoranthene-d10

Concen: 1.065 ng

RT: 19.27 min Scan# 1432

Delta R.T. -0.00 min

Lab File: BE093508.D

Acq: 21 Jul 2017 14:21

Tgt Ion:212 Resp: 267288

Ion Ratio Lower Upper

212 100

106 3.2 2.4 3.6

104 1.8 1.6 2.4

