
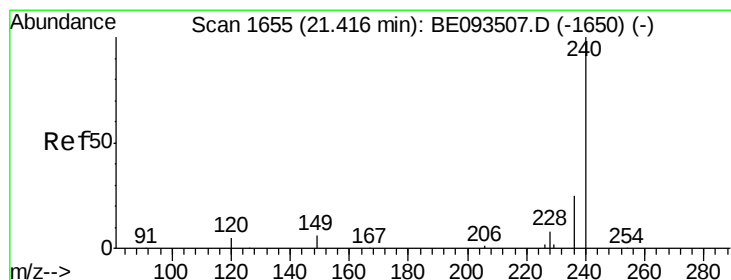
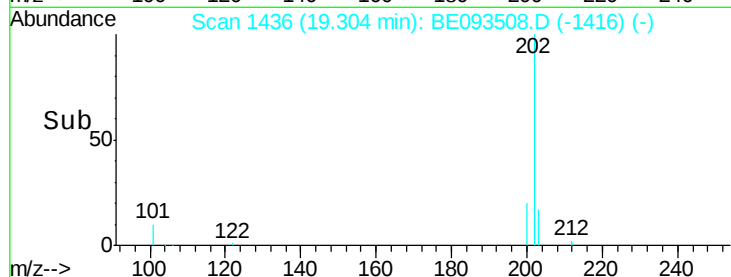
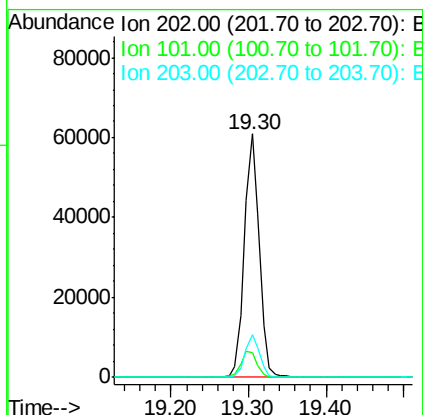


#26
 Fluoranthene
 Concen: 1.137 ng
 RT: 19.30 min Scan# 1436
 Delta R.T. -0.00 min
 Lab File: BE093508.D
 Acq: 21 Jul 2017 14:21

Instrument :
 BNA_E
 ClientSampleId :

Tgt Ion:202 Resp: 80831
 Ion Ratio Lower Upper
 202 100
 101 11.2 9.6 14.4
 203 17.0 14.4 21.6

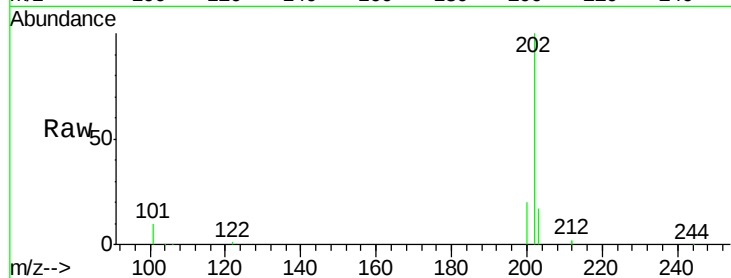

#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.42 min Scan# 1655
 Delta R.T. -0.00 min
 Lab File: BE093508.D
 Acq: 21 Jul 2017 14:21

Tgt Ion:240 Resp: 32468
 Ion Ratio Lower Upper
 240 100
 120 6.0 4.6 7.0
 236 25.0 20.8 31.2

