

#30

Benzo(a)anthracene

Concen: 0.924 ng

RT: 21.39 min Scan# 1653

Delta R.T. -0.00 min

Lab File: BE093508.D





Acq: 21 Jul 2017 14:21

Instrument :

BNA_E

ClientSampleId :

Tgt Ion:	228	Resp:	80950
Ion	Ratio	Lower	Upper
228	100		
226	27.1	19.7	29.5
229	19.9	19.2	28.8

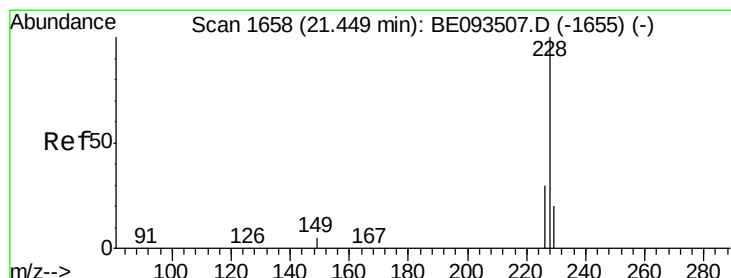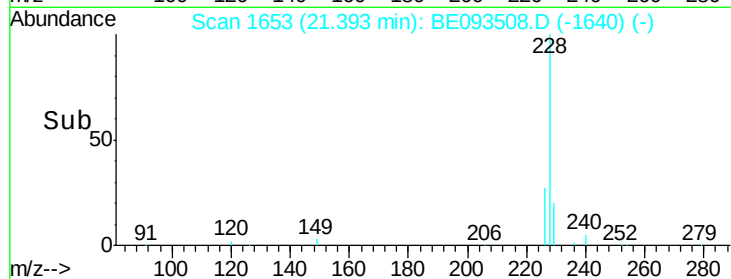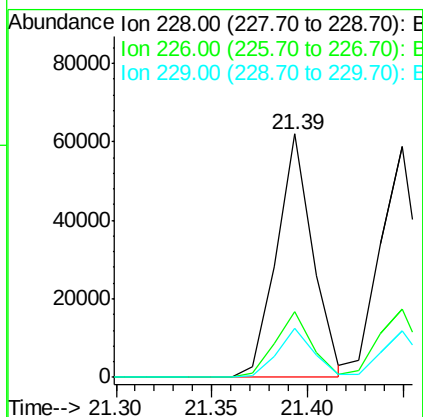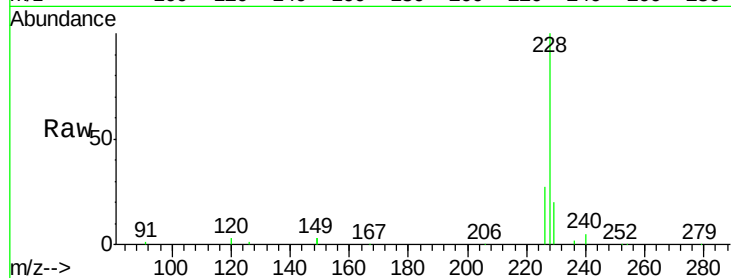

#31

Chrysene

Concen: 0.898 ng

RT: 21.45 min Scan# 1658

Delta R.T. -0.00 min

Lab File: BE093508.D

Acq: 21 Jul 2017 14:21

Tgt Ion:	228	Resp:	82338
Ion	Ratio	Lower	Upper
228	100		
226	29.4	21.5	32.3
229	20.0	18.6	28.0

