
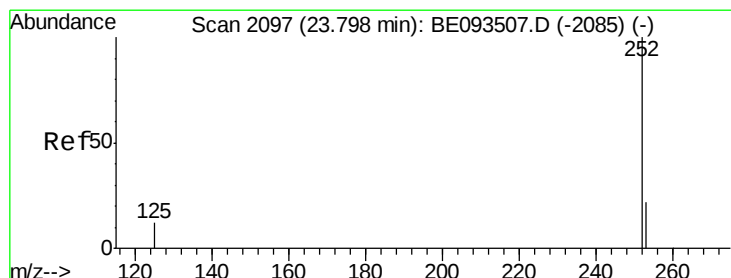
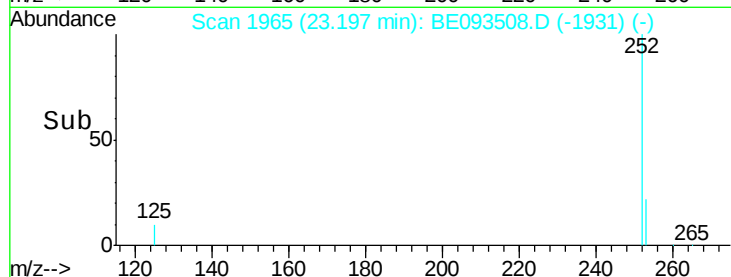
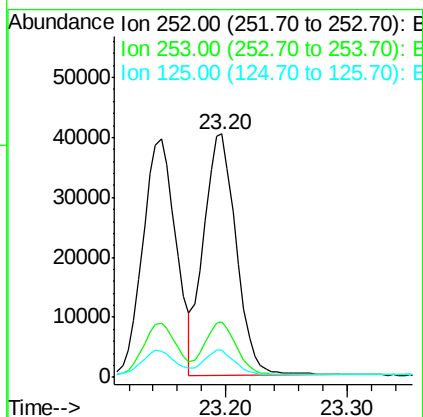


#36
Benzo(k)fluoranthene
Concen: 0.862 ng
RT: 23.20 min Scan# 1965
Delta R.T. 0.00 min
Lab File: BE093508.D
Acq: 21 Jul 2017 14:21

Instrument :
BNA_E
ClientSampleId :

Tgt Ion:252 Resp: 75177
Ion Ratio Lower Upper
252 100
253 22.6 20.3 30.5
125 11.1 12.2 18.4#

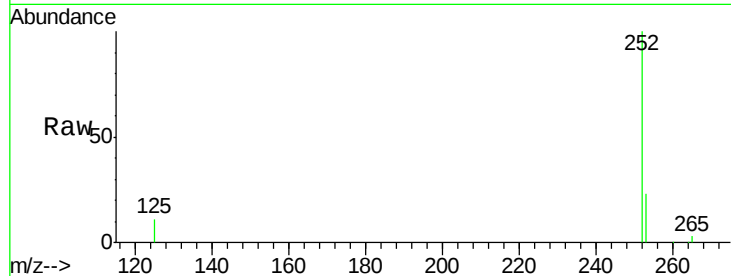

#37
Benzo(a)pyrene
Concen: 0.913 ng
RT: 23.80 min Scan# 2098
Delta R.T. 0.00 min
Lab File: BE093508.D
Acq: 21 Jul 2017 14:21

Tgt Ion:252 Resp: 70465
Ion Ratio Lower Upper
252 100
253 22.9 19.9 29.9
125 13.0 14.6 21.8#

