

#38

Dibenzo(a,h)anthracene

Concen: 0.893 ng

RT: 26.57 min Scan# 2703

Delta R.T. 0.00 min


Lab File: BE093508.D

Acq: 21 Jul 2017 14:21

Instrument :

BNA_E

ClientSampleId :

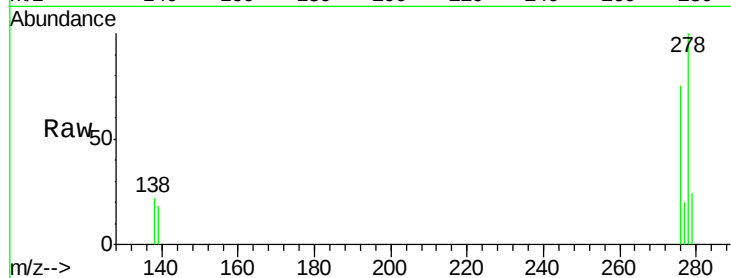




Tgt Ion:278 Resp: 66976

Ion Ratio Lower Upper

278 100

139 17.7 21.4 32.0#

279 23.9 22.2 33.2

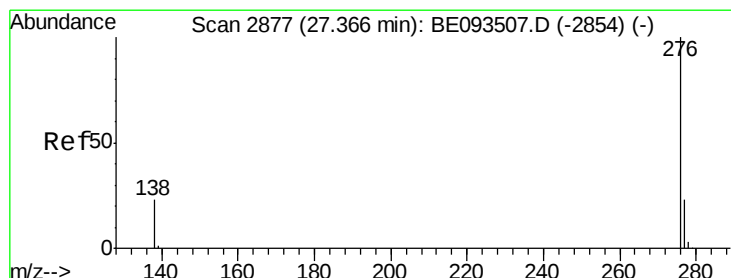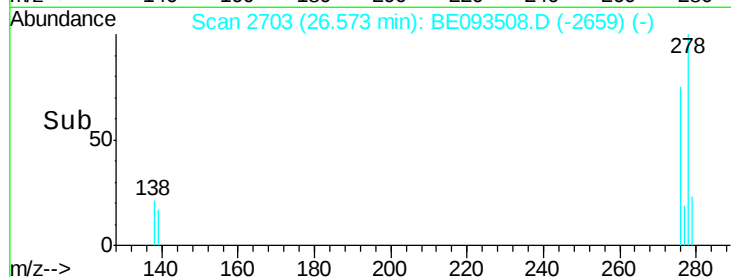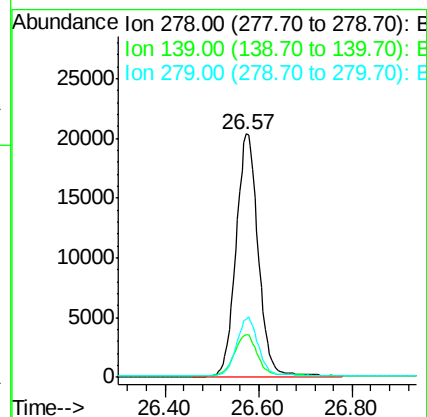

#39

Benzo(g,h,i)perylene

Concen: 0.877 ng

RT: 27.37 min Scan# 2877

Delta R.T. 0.00 min

Lab File: BE093508.D

Acq: 21 Jul 2017 14:21

Tgt Ion:276 Resp: 66412

Ion Ratio Lower Upper

276 100

277 24.2 21.2 31.8

138 22.9 24.5 36.7#

