
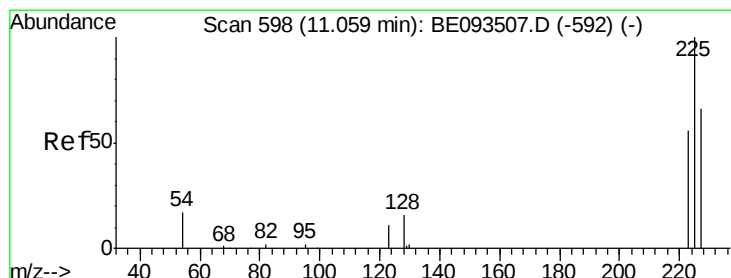
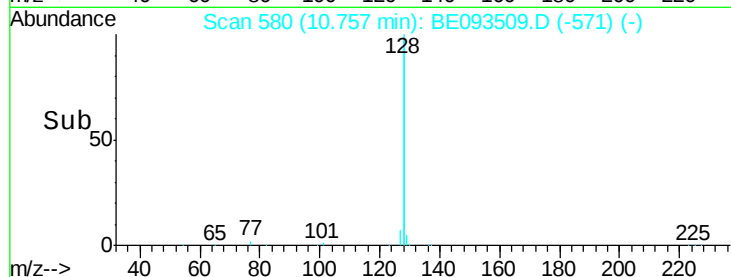
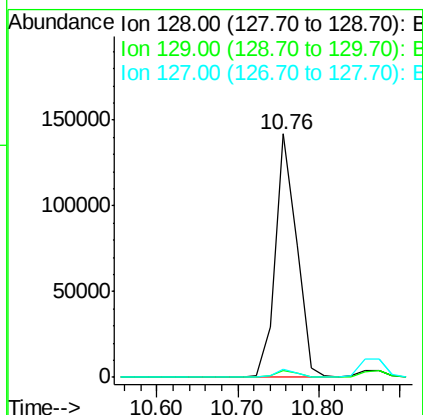


#9
Naphthalene
Concen: 1.737 ng
RT: 10.76 min Scan# 580
Delta R.T. 0.00 min
Lab File: BE093509.D
Acq: 21 Jul 2017 14:57

Instrument :
BNA_E
ClientSampleId :

Tgt Ion:128 Resp: 254415
Ion Ratio Lower Upper
128 100
129 2.8 2.4 3.6
127 3.3 2.4 3.6

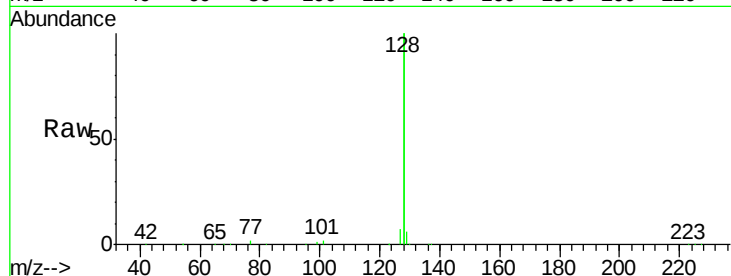

#10
Hexachlorobutadiene
Concen: 1.783 ng
RT: 11.04 min Scan# 597
Delta R.T. -0.02 min
Lab File: BE093509.D
Acq: 21 Jul 2017 14:57

Tgt Ion:225 Resp: 9912
Ion Ratio Lower Upper
225 100
223 63.3 49.7 74.5
227 65.0 50.3 75.5

