
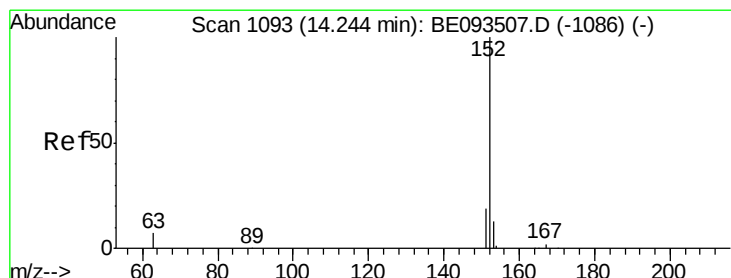
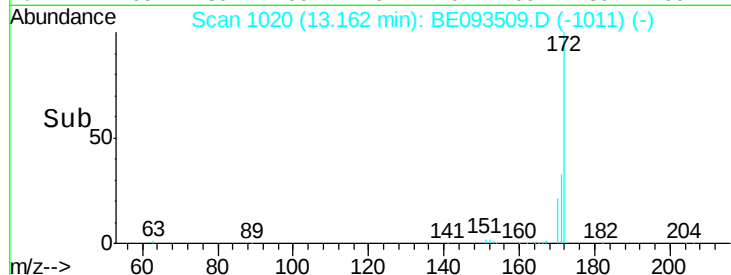
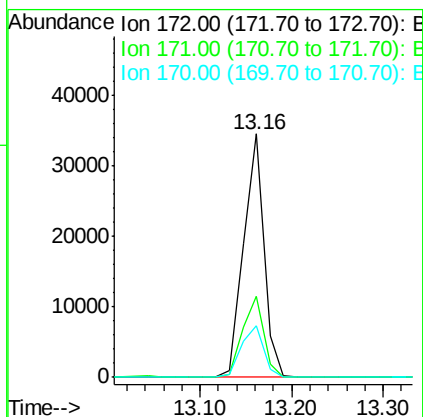


#15
2-Fluorobiphenyl
Concen: 1.559 ng
RT: 13.16 min Scan# 1020
Delta R.T. -0.00 min
Lab File: BE093509.D
Acq: 21 Jul 2017 14:57

Instrument :
BNA_E
ClientSampleId :

Tgt Ion:172 Resp: 53738
Ion Ratio Lower Upper
172 100
171 33.3 29.8 44.6
170 21.1 20.7 31.1

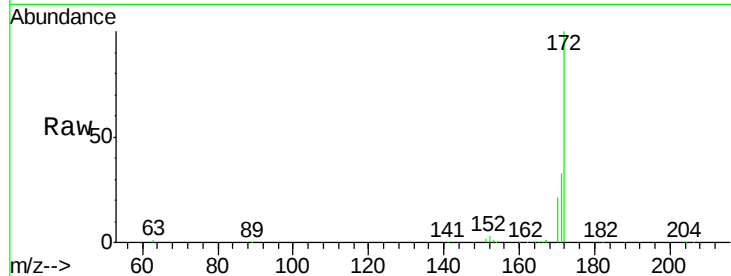

#16
Acenaphthylene
Concen: 1.987 ng
RT: 14.24 min Scan# 1093
Delta R.T. -0.00 min
Lab File: BE093509.D
Acq: 21 Jul 2017 14:57

Tgt Ion:152 Resp: 73498
Ion Ratio Lower Upper
152 100
151 19.6 4.0 6.0#
153 13.1 10.3 15.5

