

#24

Anthracene

Concen: 3.947 ng

RT: 17.37 min Scan# 1247

Delta R.T. -0.00 min

Lab File: BE093509.D

Acq: 21 Jul 2017 14:57

Instrument :

BNA_E

ClientSampleId :





Tgt Ion:178 Resp: 197240

Ion Ratio Lower Upper

178 100

176 20.9 14.6 22.0

179 13.9 12.0 18.0

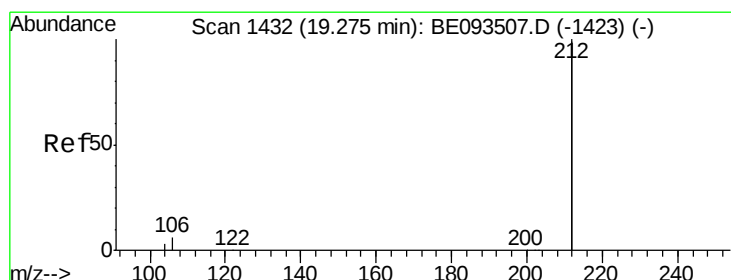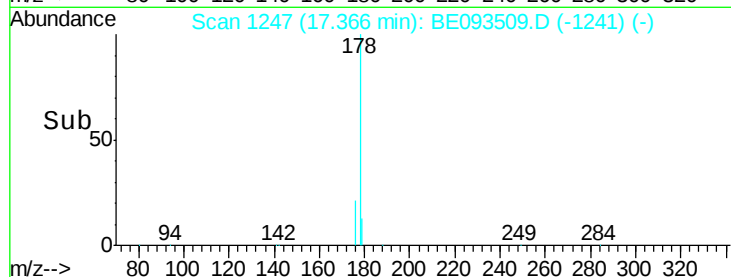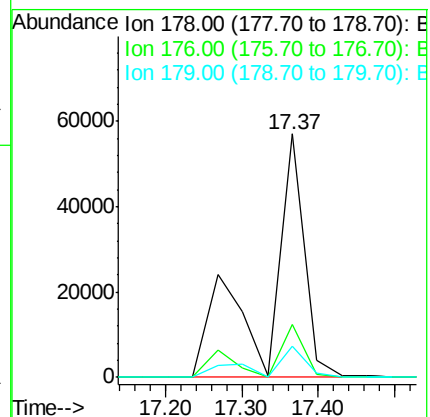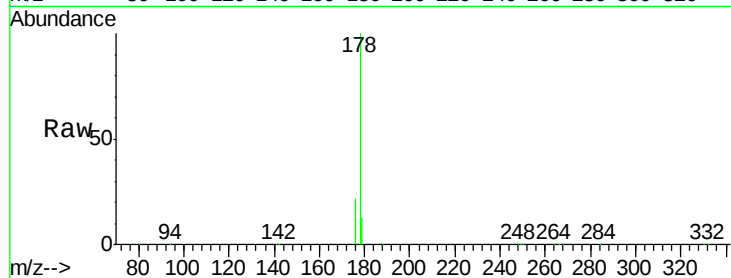

#25

Fluoranthene-d10

Concen: 2.032 ng

RT: 19.28 min Scan# 1432

Delta R.T. 0.00 min

Lab File: BE093509.D

Acq: 21 Jul 2017 14:57

Tgt Ion:212 Resp: 549302

Ion Ratio Lower Upper

212 100

106 3.3 2.4 3.6

104 1.8 1.6 2.4

