
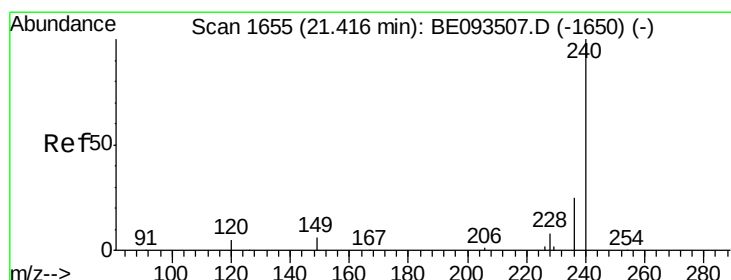
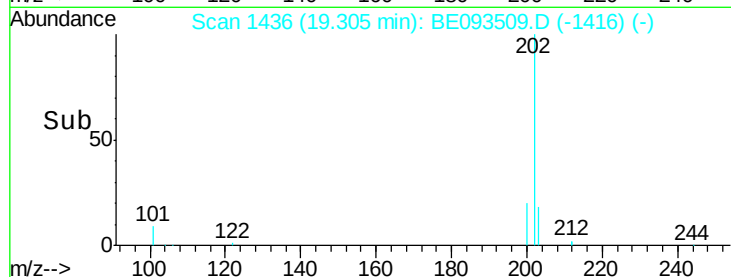
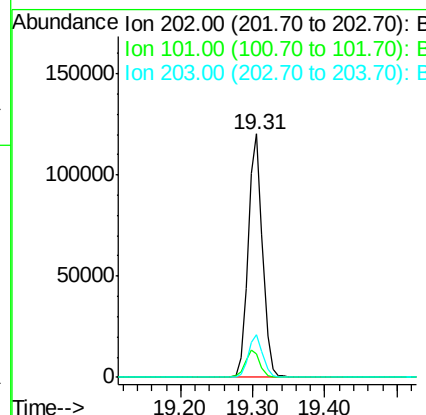


#26
 Fluoranthene
 Concen: 2.168 ng
 RT: 19.31 min Scan# 1436
 Delta R.T. 0.00 min
 Lab File: BE093509.D
 Acq: 21 Jul 2017 14:57

Instrument :
 BNA_E
 ClientSampleId :

Tgt Ion: 202 Resp: 166101
 Ion Ratio Lower Upper
 202 100
 101 11.3 9.6 14.4
 203 17.3 14.4 21.6

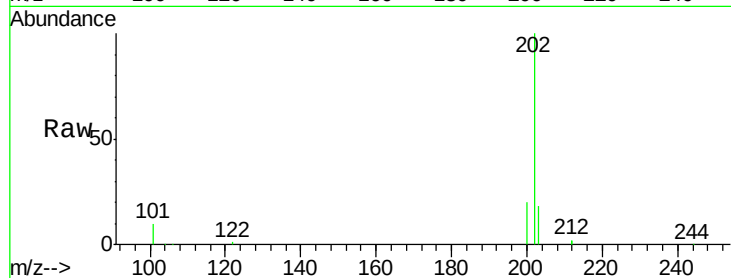

#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.42 min Scan# 1655
 Delta R.T. -0.00 min
 Lab File: BE093509.D
 Acq: 21 Jul 2017 14:57

Tgt Ion: 240 Resp: 32759
 Ion Ratio Lower Upper
 240 100
 120 5.9 4.6 7.0
 236 24.6 20.8 31.2

