

#30

Benzo(a)anthracene

Concen: 1.882 ng

RT: 21.39 min Scan# 1653

Delta R.T. -0.00 min

Lab File: BE093509.D

Acq: 21 Jul 2017 14:57

Instrument :

BNA\_E

ClientSampleId :


Tgt Ion:228 Resp: 166391

Ion Ratio Lower Upper

228 100

226 26.8 19.7 29.5




229 20.0 19.2 28.8

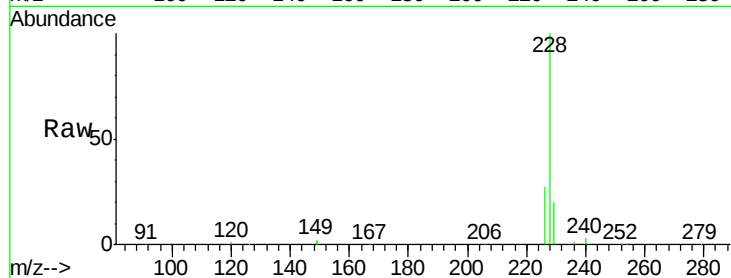

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

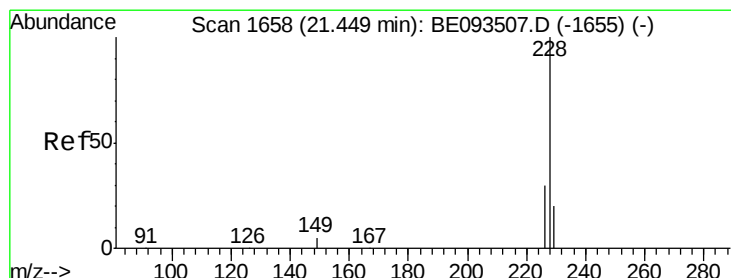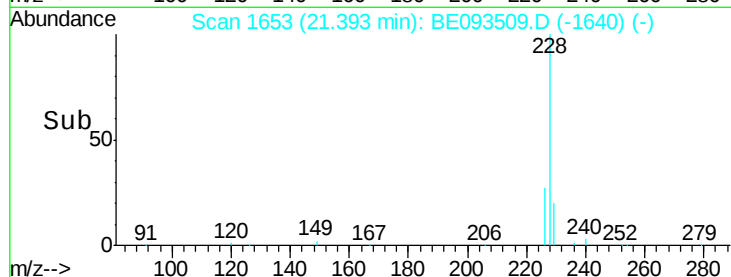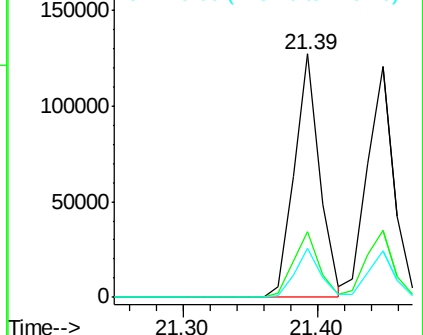

#31

Chrysene

Concen: 1.804 ng

RT: 21.45 min Scan# 1658

Delta R.T. -0.00 min

Lab File: BE093509.D

Acq: 21 Jul 2017 14:57


Tgt Ion:228 Resp: 166855

Ion Ratio Lower Upper

228 100

226 28.9 21.5 32.3

229 20.2 18.6 28.0

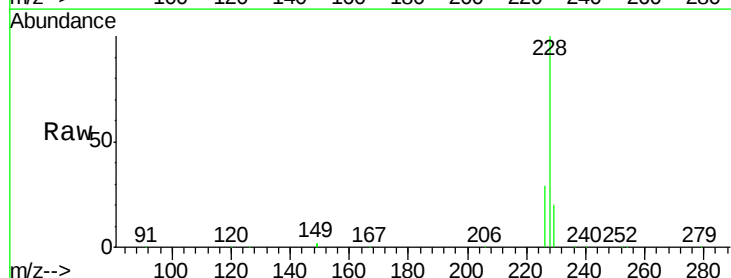

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

