

#36

Benzo(k)fluoranthene

Concen: 1.789 ng

RT: 23.19 min Scan# 1964

Delta R.T. -0.00 min

Lab File: BE093509.D

Acq: 21 Jul 2017 14:57





Instrument :

BNA_E

ClientSampleId :

Tgt Ion:252 Resp: 154329

Ion	Ratio	Lower	Upper
252	100		
253	21.7	20.3	30.5
125	10.6	12.2	18.4#

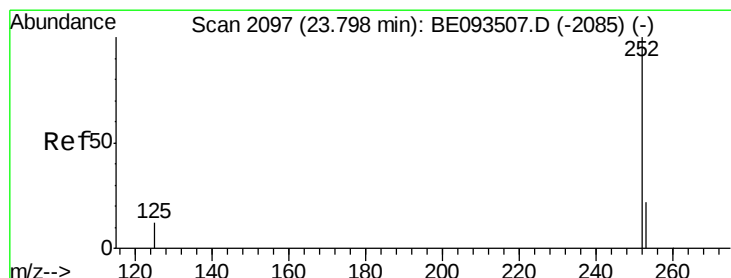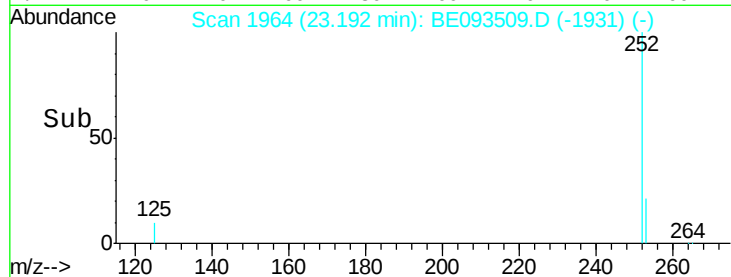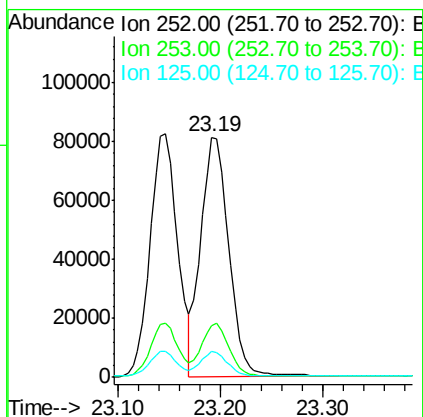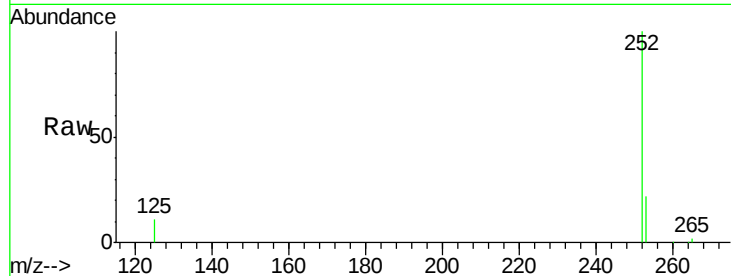

#37

Benzo(a)pyrene

Concen: 1.863 ng

RT: 23.80 min Scan# 2098

Delta R.T. 0.00 min

Lab File: BE093509.D

Acq: 21 Jul 2017 14:57

Tgt Ion:252 Resp: 142360

Ion	Ratio	Lower	Upper
252	100		
253	22.1	19.9	29.9
125	11.7	14.6	21.8#

