
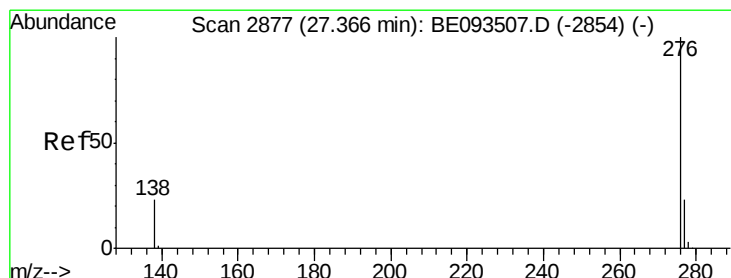
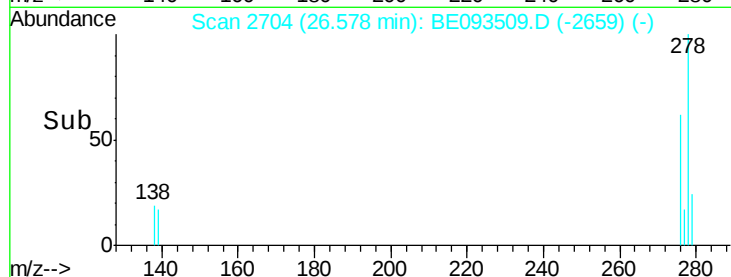
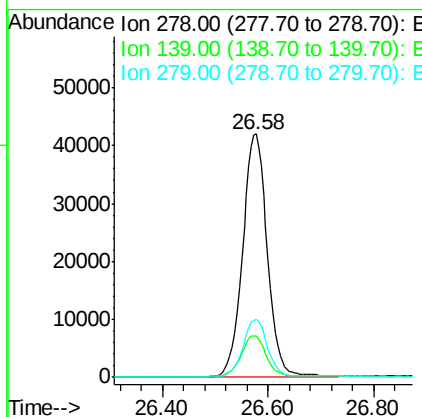


#38
Dibenzo(a,h)anthracene
Concen: 1.829 ng
RT: 26.58 min Scan# 2704
Delta R.T. 0.00 min
Lab File: BE093509.D
Acq: 21 Jul 2017 14:57

Instrument :
BNA_E
ClientSampleId :

Tgt Ion: 278 Resp: 135720
Ion Ratio Lower Upper
278 100
139 17.0 21.4 32.0#
279 24.0 22.2 33.2

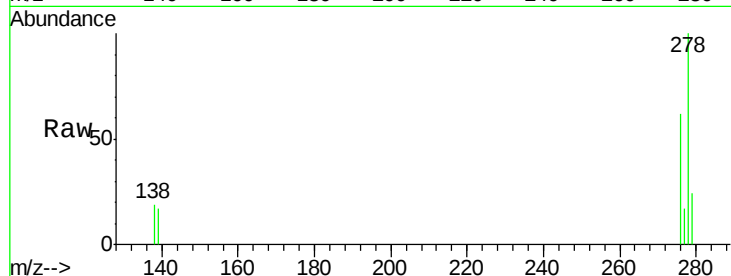

#39
Benzo(g,h,i)perylene
Concen: 1.801 ng
RT: 27.37 min Scan# 2877
Delta R.T. 0.00 min
Lab File: BE093509.D
Acq: 21 Jul 2017 14:57

Tgt Ion: 276 Resp: 134970
Ion Ratio Lower Upper
276 100
277 24.0 21.2 31.8
138 22.8 24.5 36.7#

