

#11

2-Methylnaphthalene-d10

Concen: 3.307 ng

RT: 12.30 min Scan# 826

Delta R.T. -0.00 min

Lab File: BE093510.D

Acq: 21 Jul 2017 15:36

Instrument :

BNA\_E


ClientSampled :

Tgt Ion:152 Resp: 77421

Ion Ratio Lower Upper

152 100

151 19.1 15.1 22.7

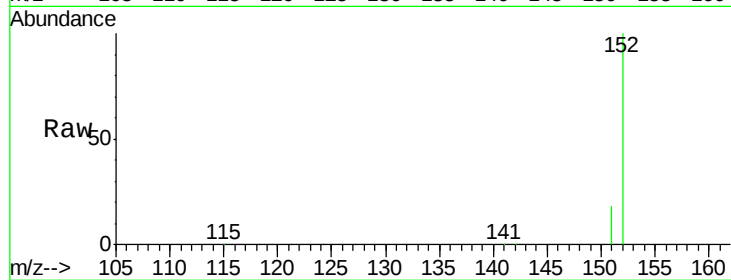

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

12.30

50000

40000



30000

20000

10000

0

Time--> 12.20 12.30 12.40

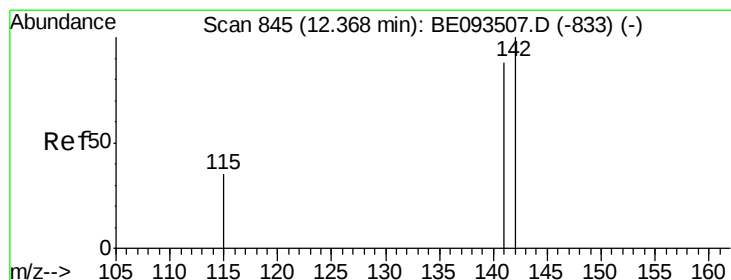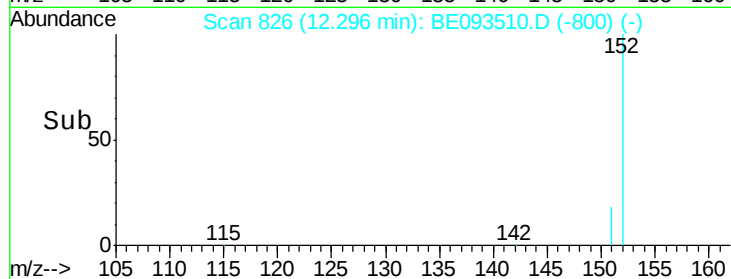

#12

2-Methylnaphthalene

Concen: 3.600 ng

RT: 12.36 min Scan# 844

Delta R.T. -0.00 min

Lab File: BE093510.D

Acq: 21 Jul 2017 15:36


Tgt Ion:142 Resp: 92957

Ion Ratio Lower Upper

142 100

141 89.1 72.6 108.8

115 37.0 32.2 48.2

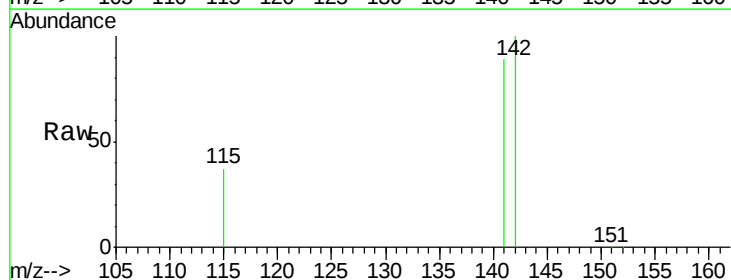

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

12.36

80000

60000

40000

20000

0

Time--> 12.30 12.40

