

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.24 min Scan# 1243

Delta R.T. -0.00 min

Lab File: BE093510.D

Acq: 21 Jul 2017 15:36

Instrument :

BNA_E

ClientSampleId :





Tgt Ion:188 Resp: 23272

Ion Ratio Lower Upper

188 100

94 17.5 11.3 16.9#

80 18.6 11.7 17.5#

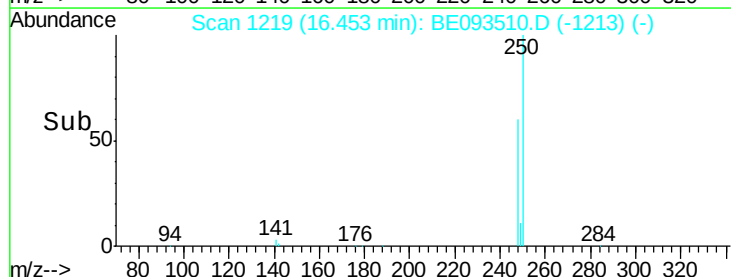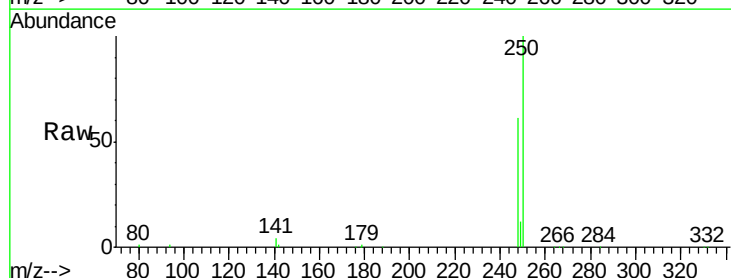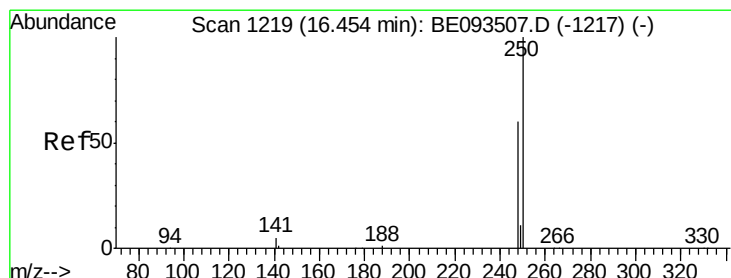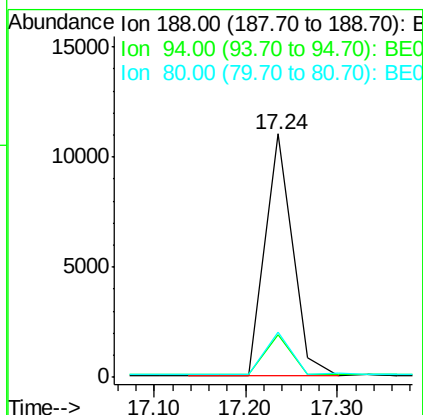

#20

4-Bromophenyl-phenylether

Concen: 2.042 ng

RT: 16.45 min Scan# 1219

Delta R.T. 0.00 min

Lab File: BE093510.D

Acq: 21 Jul 2017 15:36

Tgt Ion:248 Resp: 26063

Ion Ratio Lower Upper

248 100

250 165.1 128.0 192.0

141 6.5 12.0 18.0#

