

#24

Anthracene

Concen: 8.292 ng

RT: 17.37 min Scan# 1247

Delta R.T. -0.00 min

Lab File: BE093510.D

Acq: 21 Jul 2017 15:36

Instrument :

BNA_E

ClientSampleId :





Tgt Ion:178 Resp: 430053

Ion Ratio Lower Upper

178 100

176 20.8 14.6 22.0

179 14.0 12.0 18.0

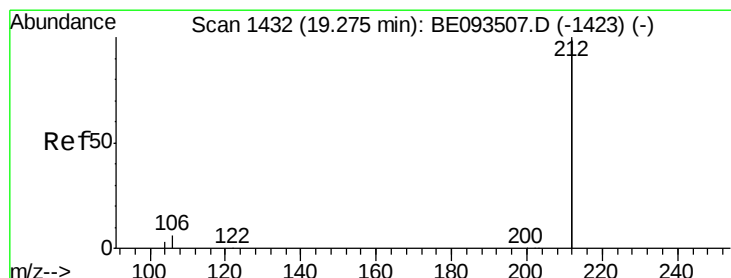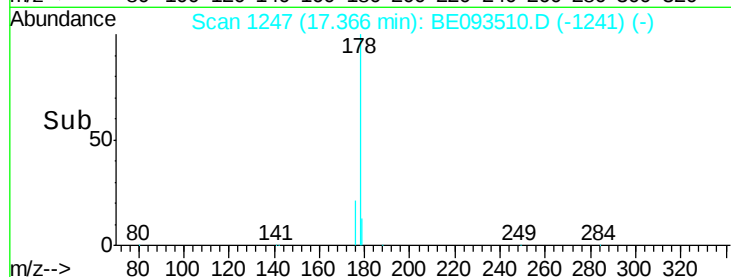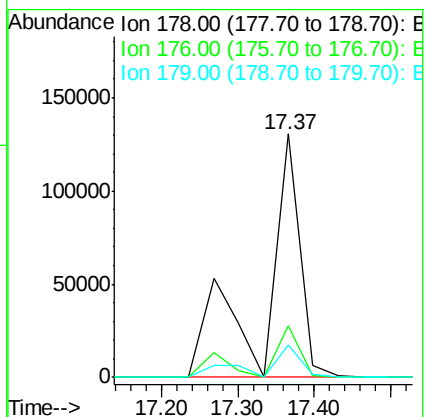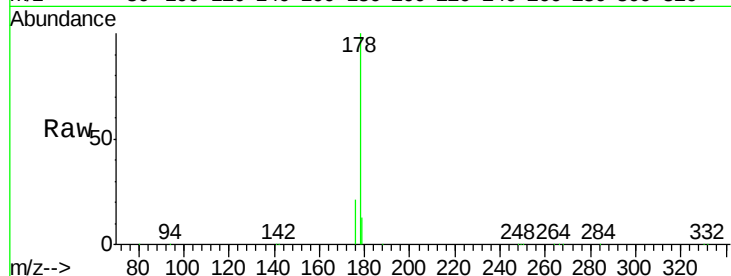

#25

Fluoranthene-d10

Concen: 3.941 ng

RT: 19.27 min Scan# 1432

Delta R.T. -0.00 min

Lab File: BE093510.D

Acq: 21 Jul 2017 15:36

Tgt Ion:212 Resp: 1105864

Ion Ratio Lower Upper

212 100

106 3.3 2.4 3.6

104 1.8 1.6 2.4

