
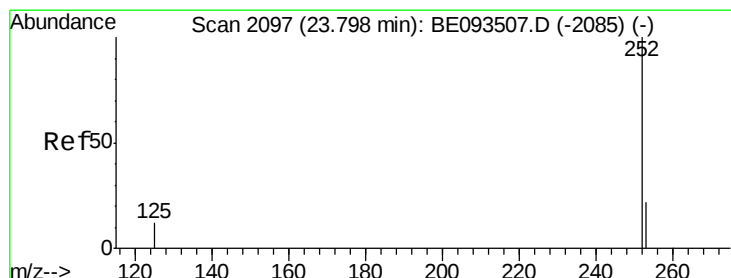
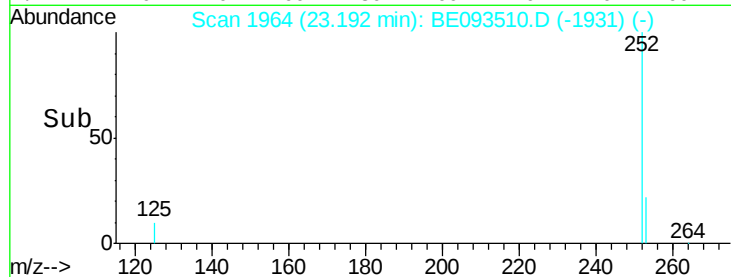
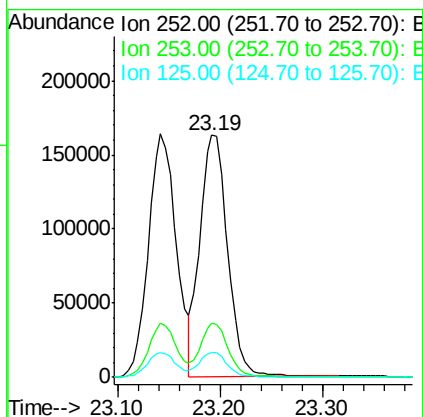


#36
Benzo(k)fluoranthene
Concen: 3.508 ng
RT: 23.19 min Scan# 1964
Delta R.T. -0.00 min
Lab File: BE093510.D
Acq: 21 Jul 2017 15:36

Instrument :
BNA_E
ClientSampleId :

Tgt Ion: 252 Resp: 305390
Ion Ratio Lower Upper
252 100
253 22.2 20.3 30.5
125 10.4 12.2 18.4#

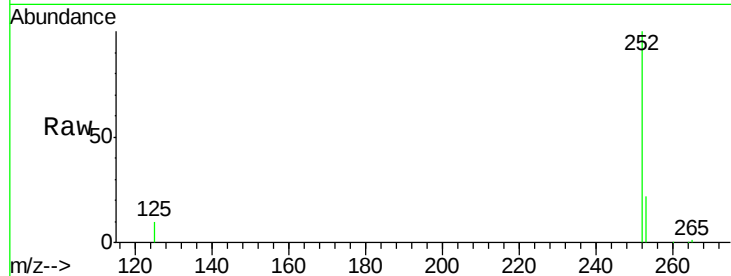

#37
Benzo(a)pyrene
Concen: 3.732 ng
RT: 23.80 min Scan# 2097
Delta R.T. -0.00 min
Lab File: BE093510.D
Acq: 21 Jul 2017 15:36

Tgt Ion: 252 Resp: 287680
Ion Ratio Lower Upper
252 100
253 22.2 19.9 29.9
125 11.3 14.6 21.8#

