

#38

Dibenzo(a,h)anthracene

Concen: 3.687 ng

RT: 26.57 min Scan# 2703

Delta R.T. 0.00 min


Lab File: BE093510.D

Acq: 21 Jul 2017 15:36




Instrument :

BNA_E

ClientSampleId :

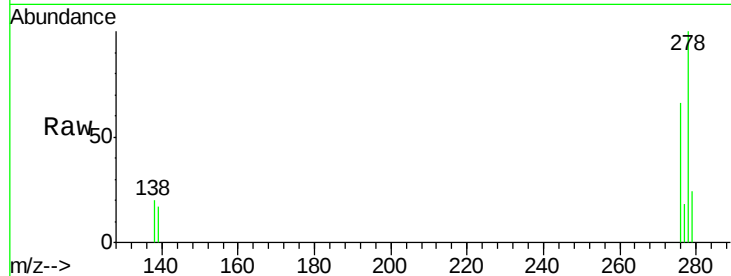

Tgt Ion:	278	Resp:	275970
Ion	Ratio	Lower	Upper
278	100		
139	16.8	21.4	32.0#
279	23.8	22.2	33.2

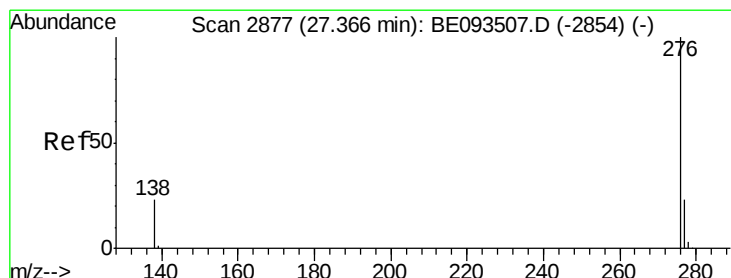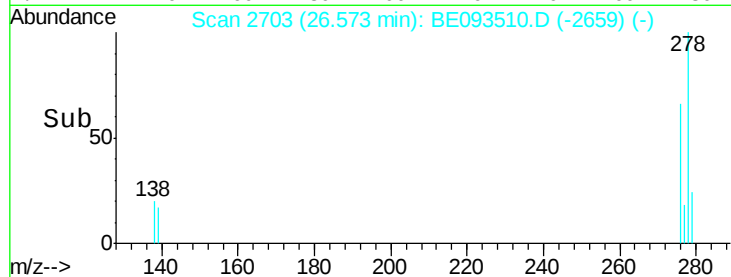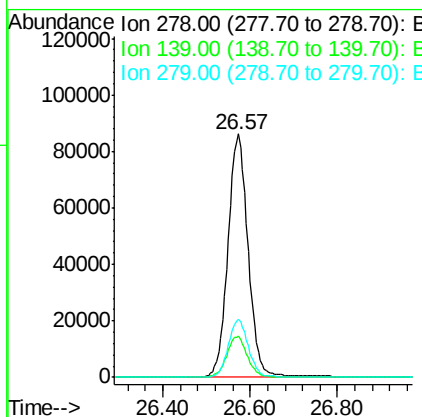

#39

Benzo(g,h,i)perylene

Concen: 3.612 ng

RT: 27.37 min Scan# 2877

Delta R.T. 0.00 min

Lab File: BE093510.D

Acq: 21 Jul 2017 15:36

Tgt Ion:	276	Resp:	273065
Ion	Ratio	Lower	Upper
276	100		
277	23.6	21.2	31.8
138	21.8	24.5	36.7#

