

#5

Phenol-d6

Concen: 0.380 ng

RT: 7.09 min Scan# 336

Delta R.T. -0.01 min

Lab File: BE093511.D

Acq: 21 Jul 2017 16:12


Instrument :

BNA_E

ClientSampleId :

Tgt Ion: 99 Resp: 5133




Ion	Ratio	Lower	Upper
99	100		
42	19.2	0.0	0.0#
71	34.0	0.0	0.0#

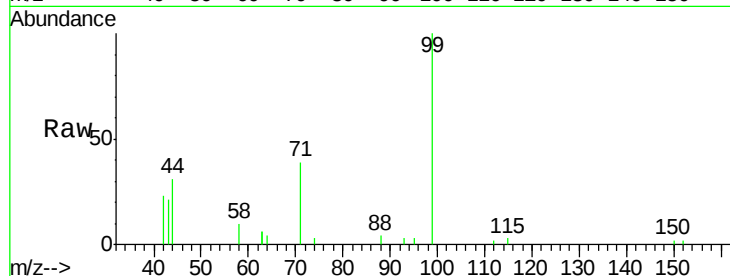

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

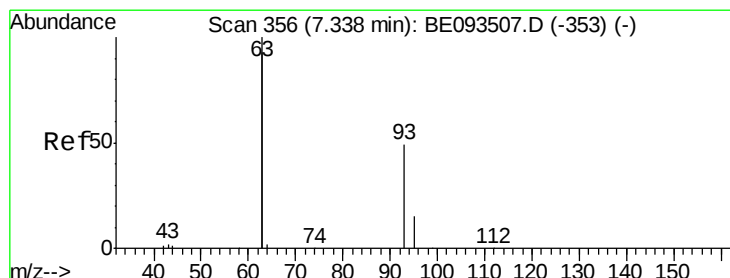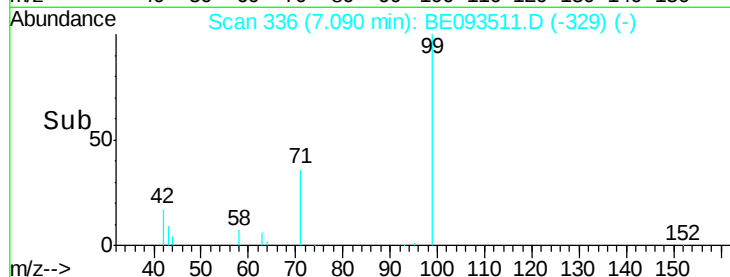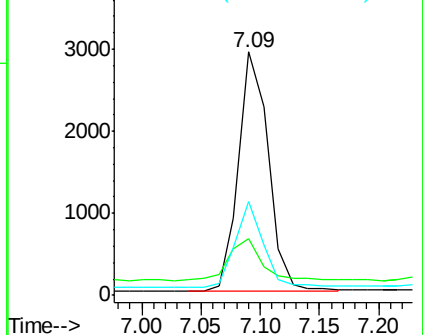

#6

bis(2-Chloroethyl)ether

Concen: 0.402 ng

RT: 7.34 min Scan# 356


Delta R.T. 0.00 min

Lab File: BE093511.D

Acq: 21 Jul 2017 16:12

Tgt Ion: 93 Resp: 4317

Ion	Ratio	Lower	Upper
93	100		
63	325.5	0.0	0.0#
95	31.7	25.4	38.0

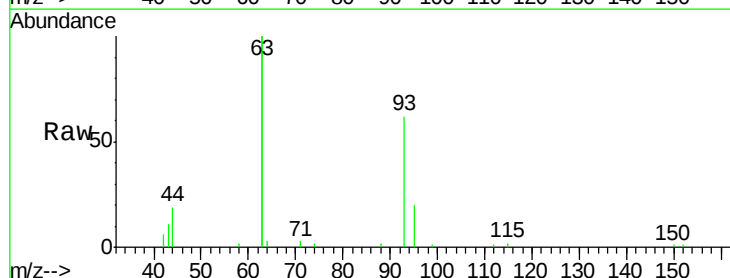

Abundance Ion 93.00 (92.70 to 93.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

Ion 95.00 (94.70 to 95.70): BE0

