





#21
Hexachlorobenzene
Concen: 0.323 ng
RT: 16.58 min Scan# 1223
Delta R.T. -0.00 min
Lab File: BE093511.D
Acq: 21 Jul 2017 16:12

Instrument :
BNA_E
ClientSampleId :

Tgt Ion: 284 Resp: 2795
Ion Ratio Lower Upper
284 100
142 0.0 0.0 0.0
249 0.0 0.0 0.0

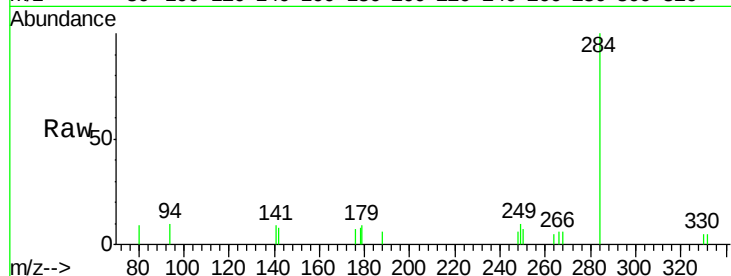


Abundance Ion 283.80 (283.50 to 284.50): E
Ion 142.00 (141.70 to 142.70): E
Ion 249.00 (248.70 to 249.70): E

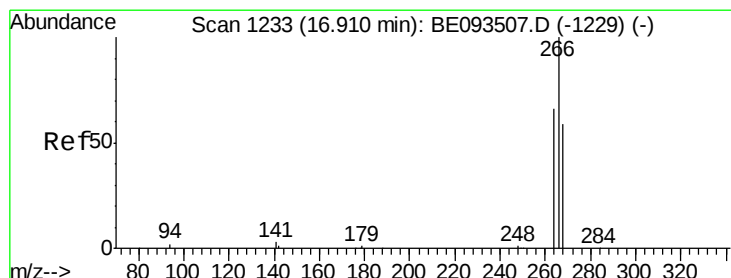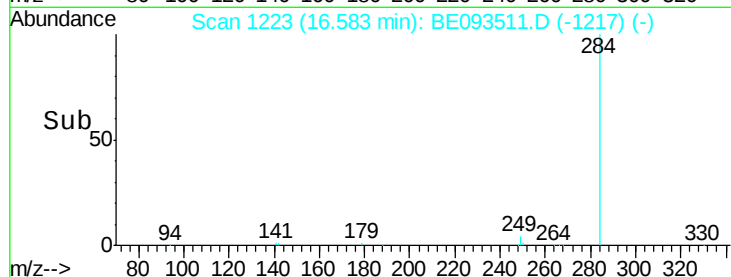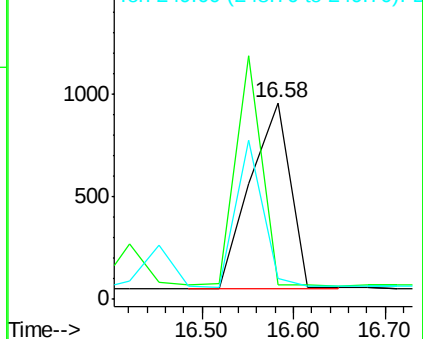

#22
Pentachlorophenol
Concen: 0.395 ng
RT: 16.91 min Scan# 1233
Delta R.T. -0.00 min
Lab File: BE093511.D
Acq: 21 Jul 2017 16:12

Tgt Ion: 266 Resp: 1414
Ion Ratio Lower Upper
266 100
264 68.5 56.0 84.0
268 67.3 52.0 78.0

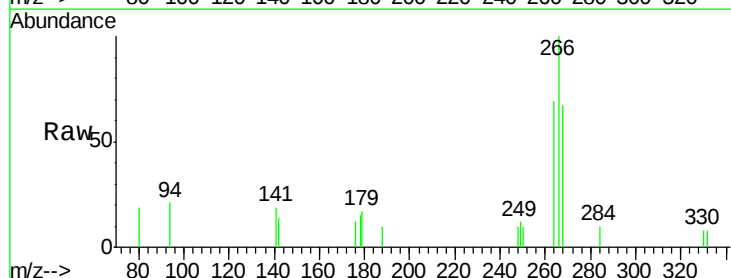

Abundance Ion 266.00 (265.70 to 266.70): E
Ion 264.00 (263.70 to 264.70): E
Ion 268.00 (267.70 to 268.70): E

