

#24

Anthracene

Concen: 0.602 ng

RT: 17.37 min Scan# 1247

Delta R.T. -0.00 min

Lab File: BE093511.D

Acq: 21 Jul 2017 16:12

Instrument :

BNA_E

ClientSampleId :


Tgt Ion:178 Resp: 48158

Ion Ratio Lower Upper

178 100

176 12.1 14.6 22.0#




179 14.0 12.0 18.0

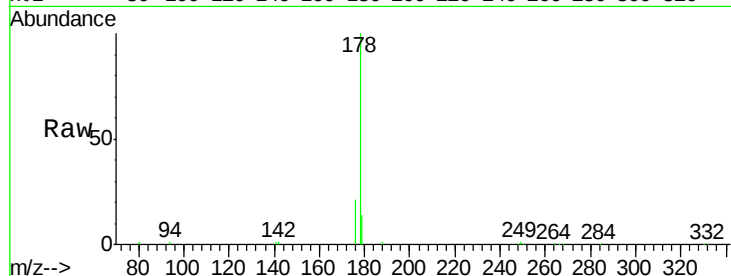

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

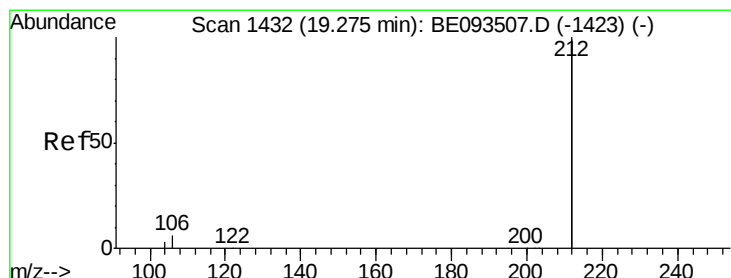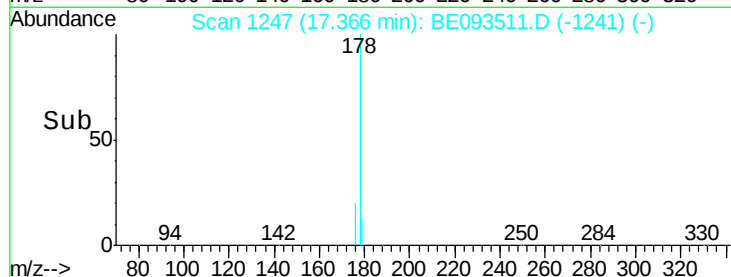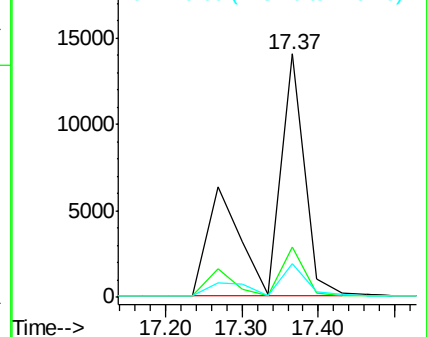

#25

Fluoranthene-d10

Concen: 0.348 ng

RT: 19.28 min Scan# 1432

Delta R.T. 0.00 min

Lab File: BE093511.D

Acq: 21 Jul 2017 16:12


Tgt Ion:212 Resp: 127942

Ion Ratio Lower Upper

212 100

106 3.2 2.4 3.6

104 1.8 1.6 2.4

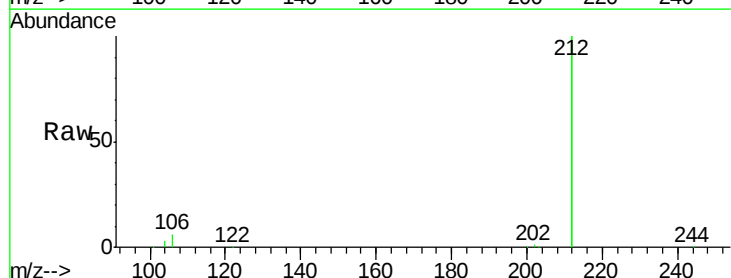

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

