

#30

Benzo(a)anthracene

Concen: 0.386 ng

RT: 21.39 min Scan# 1653

Delta R.T. -0.00 min

Lab File: BE093511.D

Acq: 21 Jul 2017 16:12

Instrument :

BNA_E

ClientSampleId :





Tgt Ion:228 Resp: 38752

Ion Ratio Lower Upper

228 100

226 26.1 19.7 29.5

229 19.5 19.2 28.8

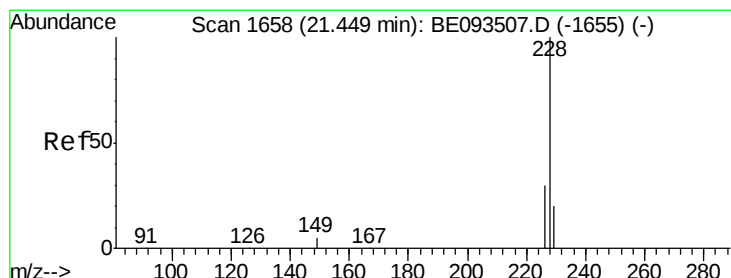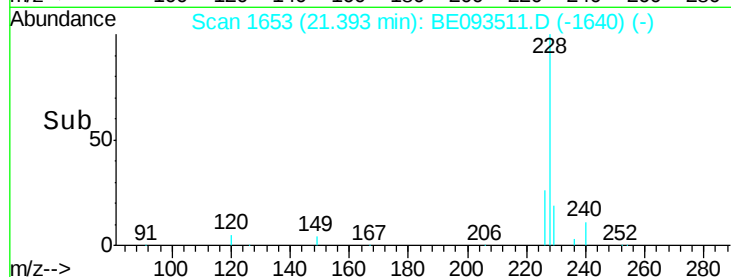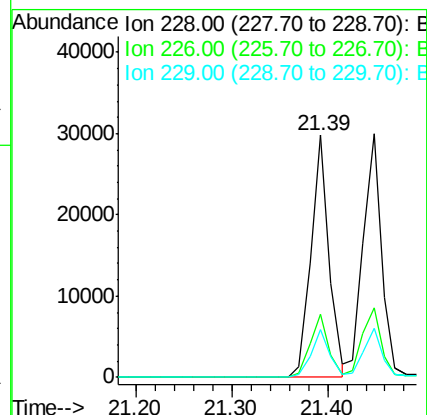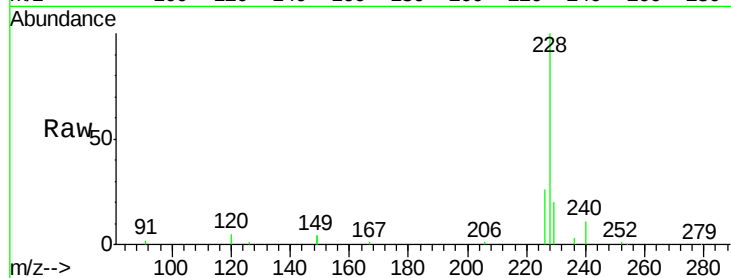

#31

Chrysene

Concen: 0.402 ng

RT: 21.45 min Scan# 1658

Delta R.T. -0.00 min

Lab File: BE093511.D

Acq: 21 Jul 2017 16:12

Tgt Ion:228 Resp: 39966

Ion Ratio Lower Upper

228 100

226 28.5 21.5 32.3

229 20.0 18.6 28.0

