

#36

Benzo(k)fluoranthene

Concen: 0.399 ng

RT: 23.14 min Scan# 1953

Delta R.T. -0.05 min

Lab File: BE093511.D

Acq: 21 Jul 2017 16:12

Instrument :

BNA_E

ClientSampleId :


Tgt Ion:252 Resp: 36673

Ion Ratio Lower Upper

252 100

253 22.3 20.3 30.5




125 12.4 12.2 18.4

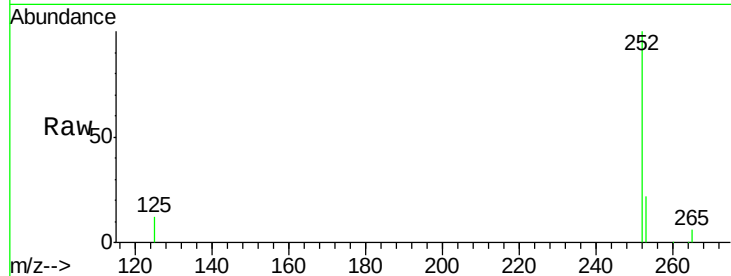

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

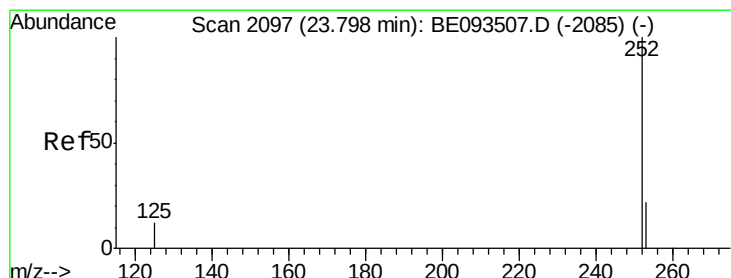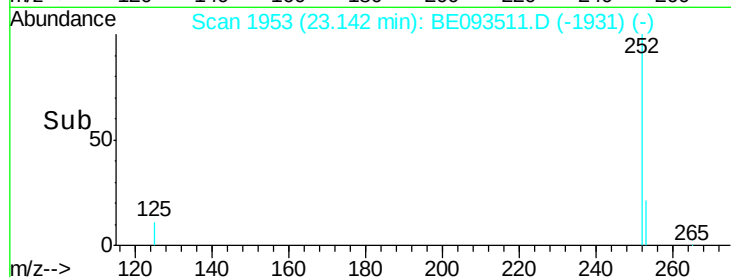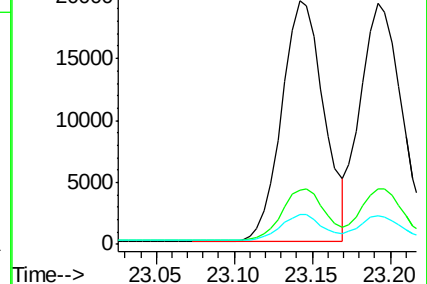

#37

Benzo(a)pyrene

Concen: 0.382 ng

RT: 23.80 min Scan# 2097

Delta R.T. -0.00 min

Lab File: BE093511.D

Acq: 21 Jul 2017 16:12


Tgt Ion:252 Resp: 33058

Ion Ratio Lower Upper

252 100

253 23.7 19.9 29.9

125 13.9 14.6 21.8#

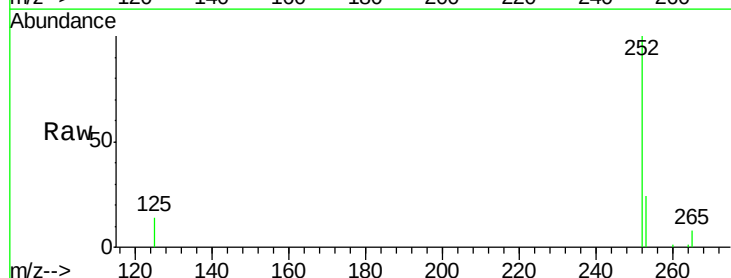

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

