
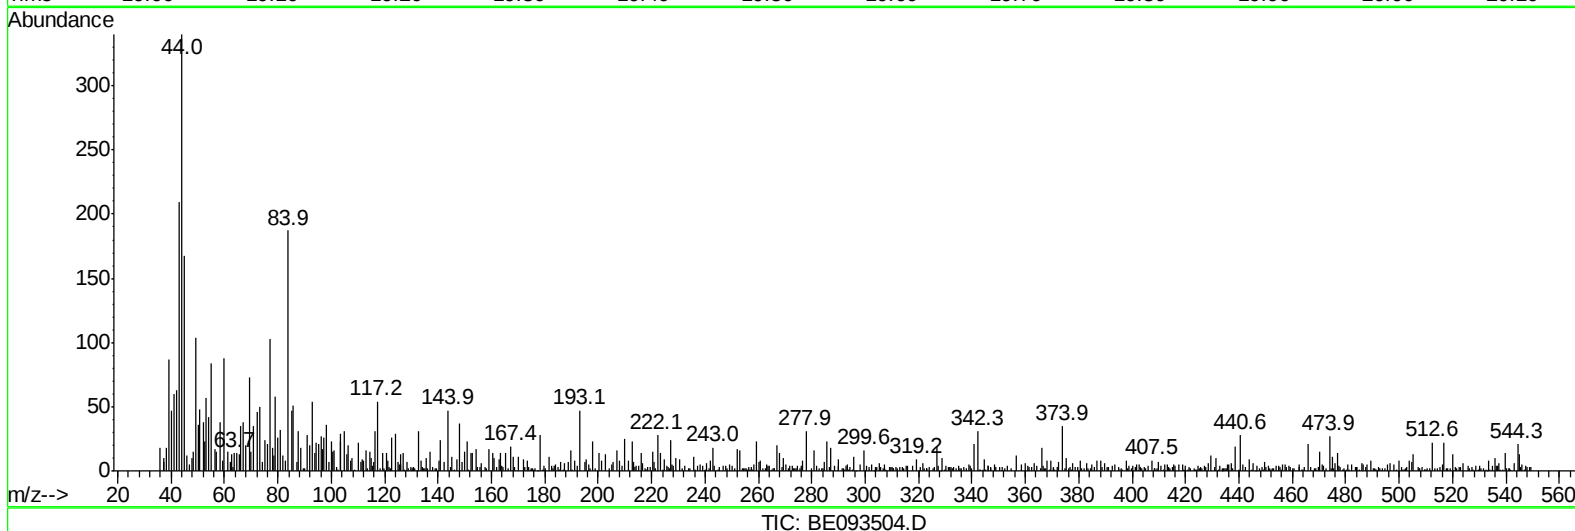


Data Path : Z:\HPCHEM1\BNA E\DATA\BE072117\
Data File : BE093504.D
Acq On : 21 Jul 2017 11:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 22 04:35:28 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 18 13:33:22 2017
Response via : Initial Calibration

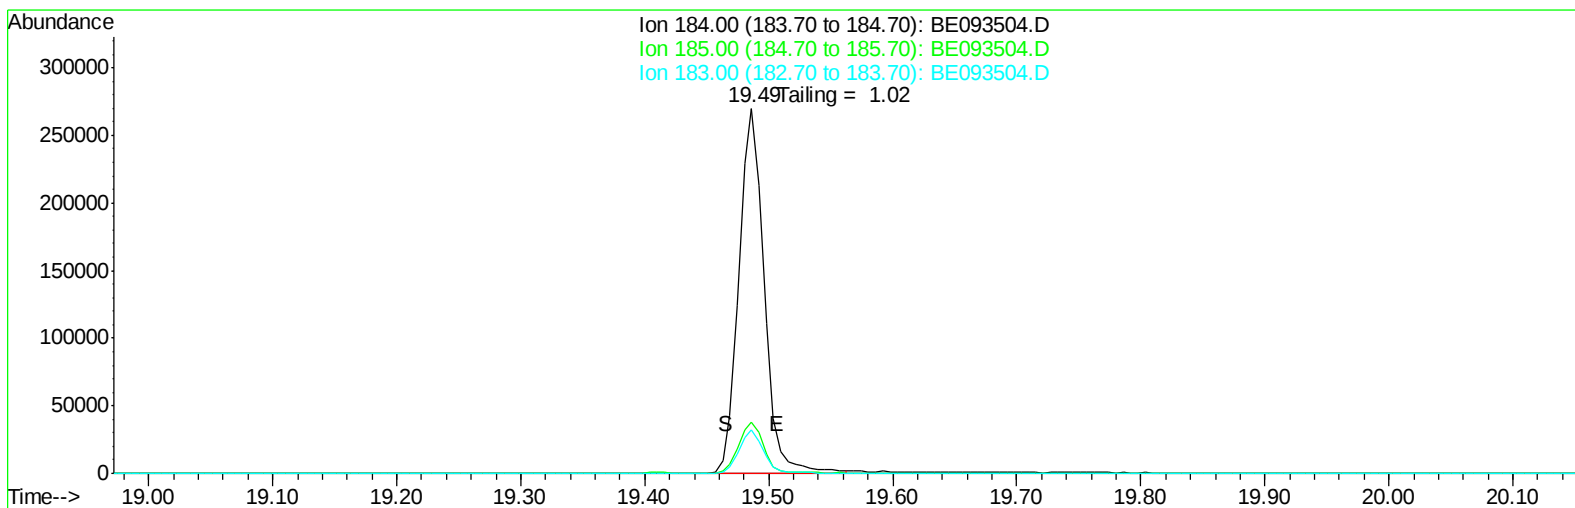

TIC: BE093504.D

(76) Benzidine



12.453min (+0.020) 10.17ng

response 4

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	80.00#
183.00	12.20	120.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE072117\
Data File : BE093504.D
Acq On : 21 Jul 2017 11:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 22 04:35:28 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 18 13:33:22 2017
Response via : Initial Calibration

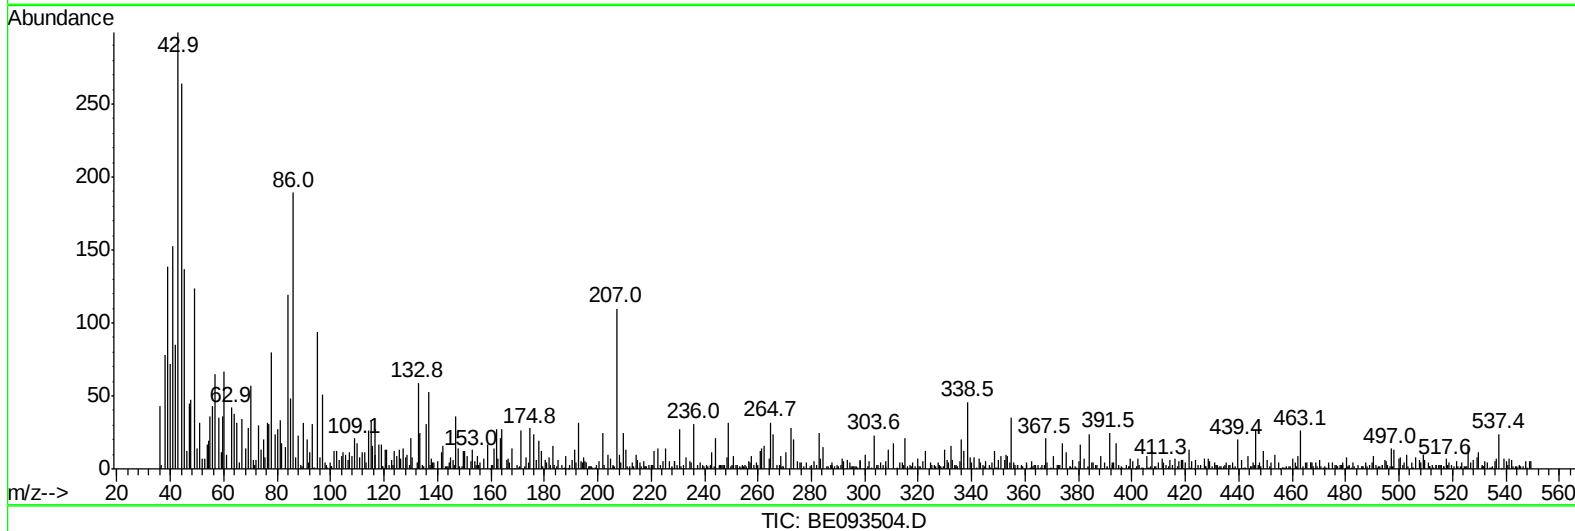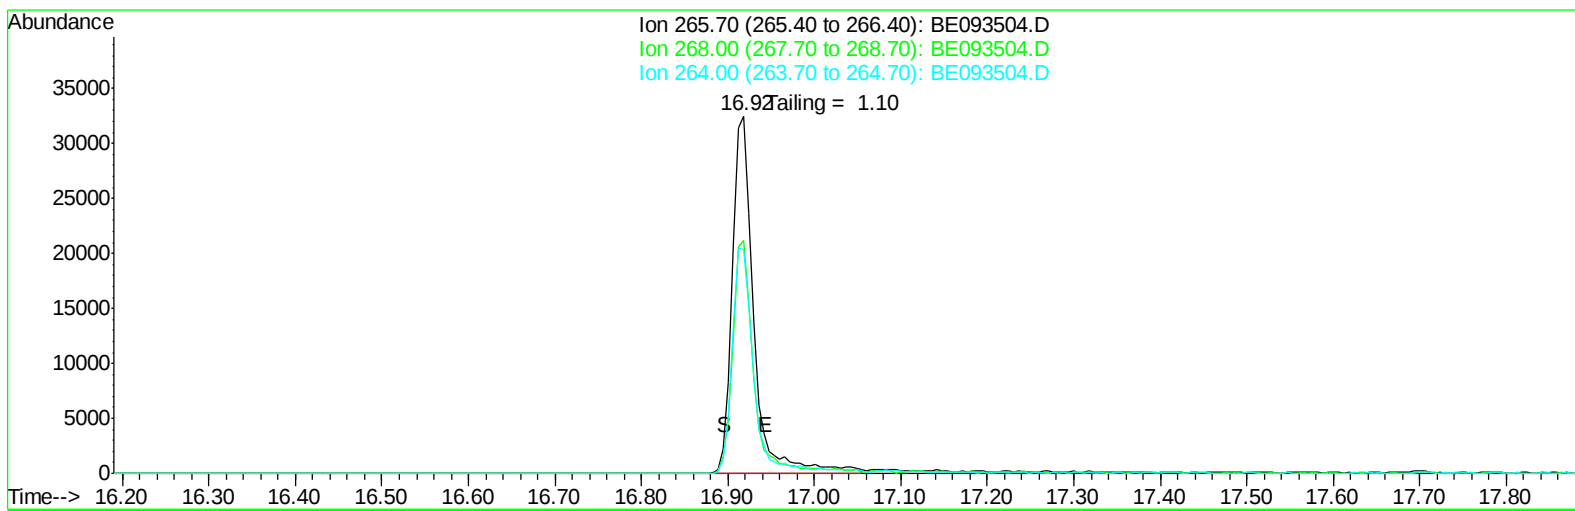

(69) Pentachlorophenol (C)

10.943min (+0.022) 364.08ng

response 22

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	50.00#
264.00	64.60	162.50#
0.00	0.00	0.00